Anritsu

MS8604A
Digital Mobile Radio Transmitter Tester
Operation Manual
Vol. 2

(714) 540-0169 Fax (714) 540-5417

Serviced By:
Excalibur Engineering Inc.

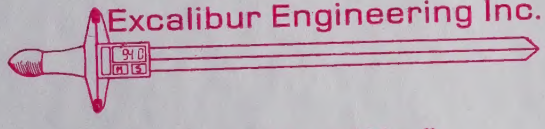

"On Time, Your Way"

3198-C Airport Loop Dr. • Costa Mesa, CA 92626
Buy • Sell • Rent • Lease

MS8604A
Digital Mobile Radio Transmitter Tester
Operation Manual
Vol. 2

(GPIB Remote Control)

Third Edition

Read this manual before using the equipment.
Keep this manual with the equipment.

Measuring Instruments Division
Measurement Group

ANRITSU CORPORATION

SEP.
1998

Document No.: M-W0682AE-3.0

MP MASTER
MA28380

ERRATA

Rev. 3.1 (1/1)

MS8604A Operation Manual vol.2 (GPIB Remote Control)

The following revisions were made after the third edition of the MS8604A Operation Manual vol.2 was issued. Please read the column on the right for the changes to the items in the column on the left.

PAGE	FOR	READ
P.6-79	**OBW?** **Response** a , f Transfers the data without suffix code as if represented in units of Hz	 Transfers the data without suffix code as if represented in units of kHz
P.6-80	**OBWFREQ?** **Response** b , f Transfers the data without suffix code as if represented in units of Hz	 Transfers the data without suffix code as if represented in units of kHz
	OCCBW? **Response** a , f Transfers the data without suffix code as if represented in units of Hz	 Transfers the data without suffix code as if represented in units of kHz
P.6-86		Add followings;

PVECTSYM? **Peak Vector Symbol**

■ Function — Output the peak vector symbol of the measurement result.

Header	Program command	Query	Response
PVECTSYM	———	PVECTSYM?	s

■ Value of s — Refer to "Number of symbols"

■ Suffix code — None

■ Example — PVECTSYM?

P.6-165	RL Suffix code	Delete followings; W: W MW: mW UW: μW NW: nW PW: pW FW: fW

Digitized by the Internet Archive
in 2025

https://archive.org/details/manualsplus_06319

For Safety

WARNING



1. Always refer to the operation manual when working near locations at which the alert mark shown on the left is attached. If the operation, etc., is performed without heeding the advice in the operation manual, there is a risk of personal injury. In addition, the equipment performance may be reduced.
   Moreover, this alert mark is sometimes used with other marks and descriptions indicating other dangers.

2. When supplying power to this equipment, connect the accessory 3-pin power cord to a 3-pin grounded power outlet. If a grounded 3-pin outlet is not available, before supplying power to the equipment, use a conversion adapter and ground the green wire, or connect the frame ground on the rear panel of the equipment to ground. If power is supplied without grounding the equipment, there is a risk of receiving a severe or fatal electric shock.

Repair

WARNING ⚠

3. This equipment cannot be repaired by the user. DO NOT attempt to open the cabinet or to disassemble internal parts. Only Anritsu-trained service personnel or staff from your sales representative with a knowledge of electrical fire and shock hazards should service this equipment. There are high-voltage parts in this equipment presenting a risk of severe injury or fatal electric shock to untrained personnel. In addition, there is a risk of damage to precision parts.

Falling Over

4. This equipment should be used in the correct position. If the cabinet is turned on its side, etc., it will be unstable and may be damaged if it falls over as a result of receiving a slight mechanical shock.

For Safety

CAUTION

Changing Fuse

CAUTION ⚠

1. Before changing the fuses, ALWAYS remove the power cord from the poweroutlet and replace the blown fuses. Always use new fuses of the type and rating specified on the fuse marking on the rear panel of the cabinet.

   T 6.3 A indicates a time-lag fuse.

   There is risk of receiving a fatal electric shock if the fuses are replaced with the power cord connected.

2. Keep the power supply and cooling fan free of dust.

   Cleaning

   - Clean the power inlet regularly. If dust accumulates around the power pins, there is a risk of fire.
   - Keep the cooling fan clean so that the ventilation holes are not obstructed. If the ventilation is obstructed, the cabinet may overheat and catch fire.

3. Use two or more people to lift and move this equipment, or use a trolley. There is a risk of back injury, if this equipment is lifted by one person.

Check Terminal

4. Never input a signal of more than 10 W between the measured terminal and ground. Input of an excessive signal may damage the equipment.

Equipment Certificate

Anritsu Corporation certifies that this equipment was tested before shipment using calibrated measuring instruments with direct traceability to public testing organizations recognized by national research laboratories including the Electrotechnical Laboratory, the National Research Laboratory and the Communication Research laboratory, and was found to meet the published specifications.

Anritsu Warranty

Anritsu Corporation will repair this equipment free-of-charge if a malfunction occurs within 1 year after shipment due to a manufacturing fault, provided that this warranty is rendered void under any or all of the following conditions.

- The fault is outside the scope of the warranty conditions described in the operation manual.
- The fault is due to misoperation, misuse, or unauthorized modification or repair of the equipment by the customer.
- The fault is due to severe usage clearly exceeding normal usage.
- The fault is due to improper or insufficient maintenance by the customer.
- The fault is due to natural disaster including fire, flooding and earthquake, etc.
- The fault is due to use of non-specified peripheral equipment, peripheral parts, consumables, etc.
- The fault is due to use of a non-specified power supply or in a non-specified installation location.

In addition, this warranty is valid only for the original equipment purchaser. It is not transferable if the equipment is resold.

Anritsu Corporation will not accept liability for equipment faults due to unforeseen and unusual circumstances, nor for faults due to mishandling by the customer.

Anritsu Corporation Contact

If this equipment develops a fault, contact Anritsu Corporation or its representatives at the address in this manual.

(Blank)

'IBM' is a registered trademark of the IBM Corporation.
'HP' is a registered trademark of the Hewlett-Packard Company.
'MS-DOS' is a registered trademark of the Microsoft Corporation.
'NEC' is a registered trademark of the NEC Corporation.

MEMORY BACK-UP BATTERY REPLACEMENT

The power for memory back-up is supplied by a Poly-carbomonofluoride Lithium Battery. This battery should only be replaced by a battery of the same type; since replacement can only be made by Anritsu, contact the nearest Anritsu representative when replacement is required.

At the end of it's life, the battery should be recycled or disposed properly.

STORAGE MEDIUM

This equipment stores data and programs using Plug-in Memory cards (PMC) and backed-up memories. Data and programs may be lost due to improper use or failure. ANRITSU therefore recommends that you back-up the memory.

ANRITSU CANNOT COMPENSATE FOR ANY MEMORY LOSS.

Please pay careful attention to the following points. Do not remove the IC card and backed-up memory from equipment being accessed.

(PMC)

- Isolate the card from static electricity.
- The back-up battery in the SRAM card has a limited life; replace the battery periodically.

(Backed-up memory)

- Isolate the memory from static electricity.

Note: The battery life is about 7 years. Early battery replacement is recommended.

DISPOSING OF THE PRODUCT

The MS8604A uses chemical compound semiconductor including arsenic.

At the end it's life, the MS8604A should be recycled or disposed properly.

ABOUT THIS MANUAL

(1) Operation manual composition

The MS8604A Operation manuals are made up of the following three manuals. Use the manuals matching the usage objective.

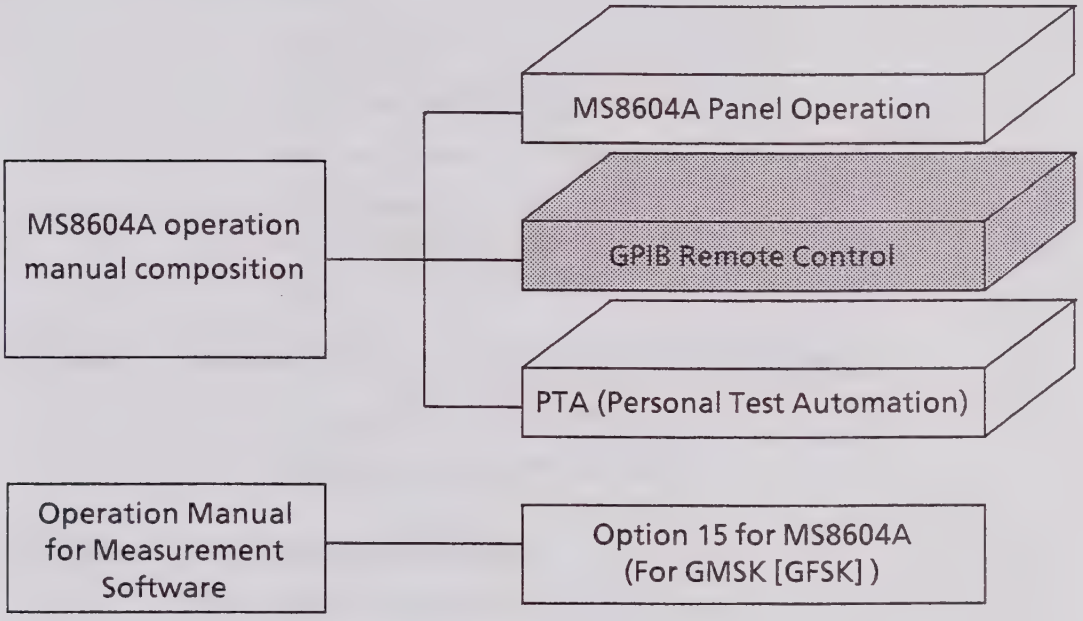

Panel Operation:	Outlines the MS8604A and describes its specifications, preparations, panels, manual (local) operation method, storage, transportation, function keys transition diagram, initial values table, and error messages.
GPIB Remote Control:	Since the MS8604A is compatible with IEEE488.2, this manual describes GPIB remote control based on IEEE488.2. The descriptions in this manual are based on N_{88}-BASIC programs using an NEC PC9800 Series personal computer for program generation reference.
PTA Personal Test Automation:	Describes how to program high-speed control and high-speed operation processing directly connected to the measurement system by high level language PTL. The program is executed by a personal computer built into the MS8604A and is called PTA (Personal Test Automation). Together with GPIB mentioned above, it promotes measurement automation.

(2) Basic Guide to GPIB (sold separately)

A "Basic Guide to GPIB" is sold separately from the operation manuals above.
This guide provides a basic knowledge of GPIB and describes the GPIB control statements written in Anritsu PACKET V computer language.

TABLE OF CONTENTS

For Safety iii

SECTION 1 GENERAL 1-1

1.1 GENERAL 1-3

1.2 Functions of GPIB 1-3

1.3 Functions of the GPIB with two ports 1-3

1.4 Examples of system configuration using GPIB 1/GPIB 2 1-4

1.5 Specifications 1-5

1.5.1 Interface function 1-5

1.5.2 Device message list 1-7

SECTION 2 CONNECTING THE BUS AND SETTING THE ADDRESS 2-1

2.1 Connecting Devices with GPIB Cables 2-3

2.2 Setting and Checking GPIB addresses 2-4

SECTION 3 DEVICE MESSAGE FORMAT 3-1

3.1 General Description 3-3

3.2 Program message format 3-3

3.3 Response message format 3-7

SECTION 4 STATUS MESSAGE 4-1

4.1 IEEE 488.2 Standard Status Model 4-4

4.2 Status Byte (STB) Register 4-6

4.2.1 ESB and MAV summary messages 4-6

4.2.2 Device-dependent summary messages 4-7

4.2.3 Reading and clearing the STB register 4-8

4.3 Enabling SRQ 4-9

4.4 Standard Event Status Register 4-10

4.4.1 Bit definition of standard event status register 4-10

4.4.2 Query error details 4-11

4.4.3 Reading, writing to and clearing the standard event status register 4-12

4.4.4 Reading, writing to and clearing the standard event status enable register 4-12

4.5 Extended Event Status Register 4-13
4.5.1 Bit definition of PTA event status register 4-14
4.5.2 Bit definition of END event status register 4-15
4.5.3 Reading, writing to and clearing the extended event status register 4-16
4.5.4 Reading, writing to and clearing the extended event status enable register 4-16
4.6 Techniques for Synchronizing MS8604A with a Controller 4-17
4.6.1 Wait for response after *OPC? query is sent 4-17
4.6.2 Wait for service request after *OPC is sent 4-18

SECTION 5 INITIAL SETTINGS 5-1
5.1 Bus Initialization by the IFC Statement 5-4
5.2 Initialization for Message Exchange by DCL and SDC Bus Commands 5-5
5.3 Device Initialization by the *RST Command 5-6
5.4 Device Initialization by the PRE/INI/IP Command 5-7
5.5 Device Status at Power-on 5-8

SECTION 6 DETAILS OF DEVICE MESSAGES 6-1
6.1 IEEE 488.2 common commands 6-7
6.2 MS8604A common commands 6-16
6.3 TX Test commands 6-44
6.4 Spectrum mode commands 6-110

SECTION 7 SAMPLE PROGRAMS 7-1
7.1 Precautions on Creating the GPIB Program 7-3
7.2 Sample Programs 7-4

SECTION 8 WAVEFORM DATA STORAGE FORMAT 8-1
8.1 Notes on Fetching the Waveform Data 8-3
8.2 Waveform Data Storage Format 8-4

APPENDIX A ASCII*CODE TABLE A-1
APPENDIX B COMPARISON TABLE OF CONTROLLERS' GPIB INSTRUCTIONS B-1

SECTION 1
GENERAL

This section outlines the GPIB functions of the MS8604A Digital Mobile Transmitter Tester.

TABLE OF CONTENTS

1.1 GENERAL 1-3

1.2 Functions of GPIB 1-3

1.3 Functions of the GPIB with two ports 1-3

1.4 Examples of system configuration using GPIB 1/GPIB 2 1-4

1.5 Specifications 1-5

1.5.1 Interface function 1-5

1.5.2 Device message list 1-7

(Blank)

1.1 GENERAL

The MS8604A Digital Mobile Transmitter Tester, when combined with an external controller, can automate your measurement system. For this purpose the MS8604A is equipped with a GPIB interface bus (IEEE std 488.2 1987) as a standard feature.

1.2 Functions of GPIB

The functions of the MS8604A GPIB are as follows:

(1) Controls all functions except the power switch and some keys including the [Local] key

(2) Reads out all setting conditions

(3) Sets the GPIB address from the panel

(4) Executes interrupts and serial polling

(5) Configures the automatic measurement system when the MS8604A is combined with a personal computer and other measuring instruments

(6) Configures the GPIB with two ports: GPIB 1 and GPIB 2

1.3 Functions of the GPIB with two ports

The MS8604A Digital Mobile Radio Transmitter Tester provides two GPIB ports, GPIB 1 and GPIB 2. The port on the GPIB 1 side is connected to an external controller to automate measurements by remote control, while the port on the GPIB 2 side is used to control peripherals such as printers, plotters, and other devices.
This Operation Manual describes the GPIB 1 port which is used for remote control. For hard-copying and other processing via the GPIB 2 port, refer to paragraph 4.7 in the Panel Operation Part of the separate Operation Manual.

1.4 Examples of system configuration using GPIB 1/GPIB 2

(1) Stand-alone type 1····· Panel operation

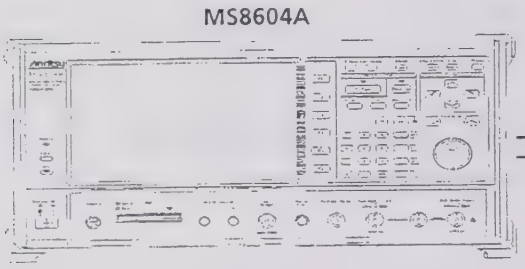

Outputs waveforms measured with the **MS8604A** to the printer.

(2) Stand-alone type 2····· Panel operation

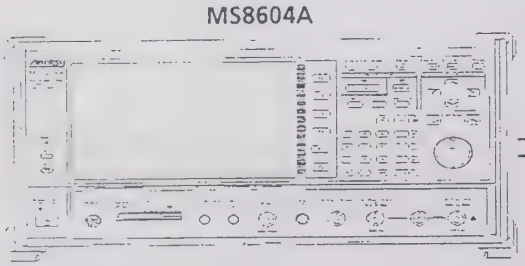

Saves parameters by the **MS8604A** on the PMC or floppy disk attached to the MC8104A Data Storage Unit.

(3) Control by the host computer

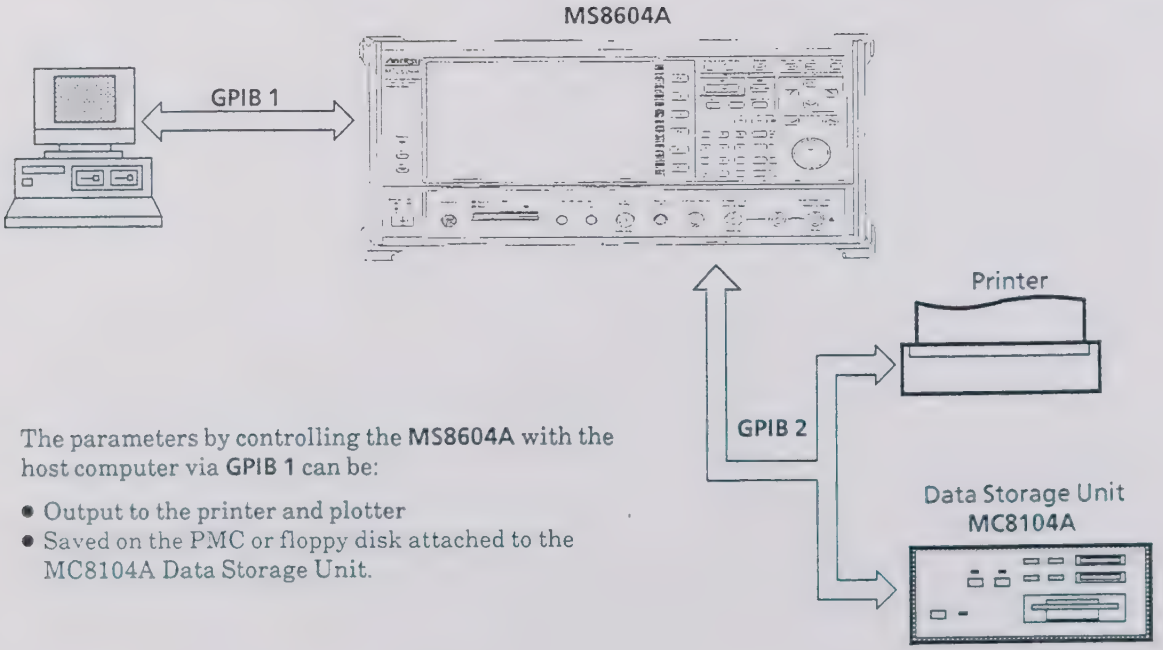

The parameters by controlling the **MS8604A** with the host computer via **GPIB 1** can be:

- Output to the printer and plotter
- Saved on the PMC or floppy disk attached to the MC8104A Data Storage Unit.

1.5 Specifications

1.5.1 Interface function

IEEE 488.2 determines the minimum required subsets for a measuring instrument from the GPIB interface functions specified in IEEE 488.1. It enables the subsets to be used for a system.

The MS8604A's GPIB 1 and GPIB 2 provide the IEEE 488.1 subsets listed in the code columns of the table below.

GPIB 1 Interface Functions

Code	Interface function
SH1	All source handshake functions are provided. Synchronizes the timing of data transmission.
AH1	All acceptor handshake functions are provided. Synchronizes the timing for receiving data.
T6	Basic talker functions are provided. The serial poll function is provided. The talk-only function is not provided. The talker can be canceled by MLA.
L4	Basic listener functions are provided. The listen-only function is not provided. The listener can be canceled by MTA.
SR1	All Service request and status byte functions are provided.
RL1	All Remote/local functions are provided. The local lockout function is provided.
PP0	Parallel poll functions are not provided.
DC1	All Device clear functions are provided.
DT1	Device trigger functions are provided.
C0	Controller functions are not provided. (When the PTA is not used)
C1 to C3 C24	Controller functions are provided. (When the PTA is used)

GPIB 2 Interface Functions

Code	Interface Function
SH1	All source handshake functions are provided. Synchronizes the timing of data transmission.
AH1	All acceptor handshake functions are provided. Synchronizes the timing for receiving data.
T6	Basic talker functions are provided. Serial poll functions are provided. The talk-only function is not provided. A talker can be canceled by MLA.
L4	Basic listener functions are provided. The listen-only function is not provided. A listener can be canceled by MTA.
SR0	Service request and status byte functions are not provided.
RL0	Remote/local functions are not provided. Local lockout functions are not provided.
PP0	Parallel poll functions are not provided.
DC0	Device clear functions are not provided.
DT0	Device trigger functions are not provided.
C1 to C4, C28	Controller functions are provided.
E2	Tri-state output

1.5.2 Device message list

A device message is a data message transmitted between the controller and device via the system interface when the bus mode (ATN line) is false (FALSE, or 0). Device messages are classified into program messages and response messages.

A program message is an ASCII data message transferred from the controller to the device. Program messages are classified into program commands and program queries. These commands and queries are listed on the following pages.

Program commands are classified into device-specific commands used exclusively to control the MS8604A, and IEEE 488.2 common commands. IEEE 488.2 common commands include commands for the MS8604A, and are also used for other measuring instruments conforming to IEEE 488.2 connected to the bus.

A program query is a command used to obtain a response message from the device. It is transferred from the controller to the device in advance, then the controller receives the response message from the device.

A response message is an ASCII data message transferred from the device to the controller. This paragraph lists response messages.

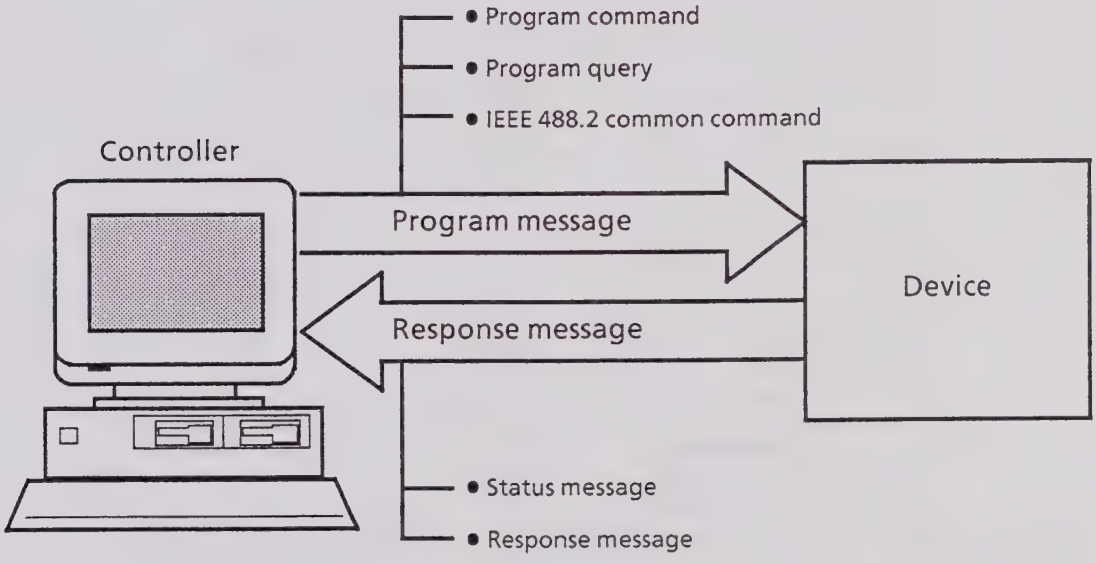

Program messages and response messages may have a suffix (units) at the end of the numeric data.

The messages explained so far are transferred via the input and output buffers of the device. The output buffer is also called the output queue. The input buffer and output buffer (queue) are briefly explained below.

Input buffer	Output queue
The input buffer is a first-in first-out (FIFO) type memory area in which data bytes (DAB [program and query messages]) to be executed are temporarily stored. A message is executed after its syntax has been analyzed. The MS8604A has a 256-byte input buffer.	The output queue is also a FIFO type memory area. All DABs (response messages) output from the device to the controller are stored in this memory until the controller reads them. The MS8604A has a 256-byte output queue.

(1) GPIB Suffix Code

The table below shows the suffixes used for the MS8604A.

Table of MS8604A Suffix codes

Classification	Unit	Suffix code
Frequency	GHz	GHZ, GZ
	MHz	MHZ, MZ
	kHz	KHZ, KZ
	Hz	HZ
	Default	HZ
Time	second	S
	m second	MS
	μ second	US
	Default	MS
Level	dB	DB
	dBm	DBM, DM
	dBμV	DBUV
	dBmV	DBMV
	dBμV (emf)	DBUVE
	Default	Determined in conformance with the set scale unit
Level	V	V
	mV	MV
	μV	UV
	Default	UV

(2) IEEE 488.2 common commands and supported commands

The table below lists 39 types of common commands specified in the IEEE 488.2 standard. IEEE 488.2 common commands which are supported by the MS8604A are indicated with ◎ symbol in the table.

Mnemonic	Command name	IEEE 488.2 Standard	MS8604A supported commands
*AAD	Accept Address Command	Optional	
*CAL?	Calibration Query	Optional	
*CLS	Clear Status Command	Mandatory	◎
*DDT	Define Device Trigger Command	Optional	
*DDT?	Define Device Trigger Query	Optional	
*DLF	Disable Listener Function Command	Optional	
*DMC	Define Macro Command	Optional	
*EMC	Enable Macro Command	Optional	
*EMC?	Enable Macro Query	Optional	
*ESE	Standard Event Status Enable Command	Mandatory	◎
*ESE?	Standard Event Status Enable Query	Mandatory	◎
*ESR?	Standard Event Status Register Query	Mandatory	◎
*GMC?	Get Macro Contents Query	Optional	
*IDN?	Identification Query	Mandatory	◎
*IST?	Individual Status Query	Optional	
*LMC?	Learn Macro Query	Optional	
*LRN?	Learn Device Setup Query	Optional	
*OPC	Operation Complete Command	Mandatory	◎
*OPC?	Operation Complete Query	Mandatory	◎
*OPT?	Option Identification Query	Optional	
*PCB	Pass Control Back Command	Mandatory if other than CO.	◎
*PMC	Purge Macro Command	Optional	
*PRE	Parallel Poll Register Enable Command	Optional	
*PRE?	Parallel Poll Register Enable Query	Optional	
*PSC	Power On Status Clear Command	Optional	◎
*PSC?	Power On Status Clear Query	Optional	◎
*PUD	Protected User Data Command	Optional	
*PUD?	Protected User Data Query	Optional	
*RCL	Recall Command	Optional	
*RDT	Resource Description Transfer Command	Optional	
*RDT?	Resource Description Transfer Query	Optional	
*RST	Reset Command	Mandatory	◎
*SAV	Save Command	Optional	
*SRE	Service Request Enable Command	Mandatory	◎
*SRE?	Service Request Enable Query	Mandatory	◎

Mnemonic	Command name	IEEE 488.2 Standard	MS8604A supported commands
*STB?	Read Status Byte Query	Mandatory	◎
*TRG	Trigger Command	Mandatory if DT1	◎
*TST?	Self Test Query	Mandatory	◎
*WAI	Wait to Continue Command	Mandatory	◎

Note: The first letter of IEEE 488.2 common commands is always *.

(3) Status messages

The diagram below shows the structure of service-request summary messages for the status byte register (STB) used with the MS8604A.

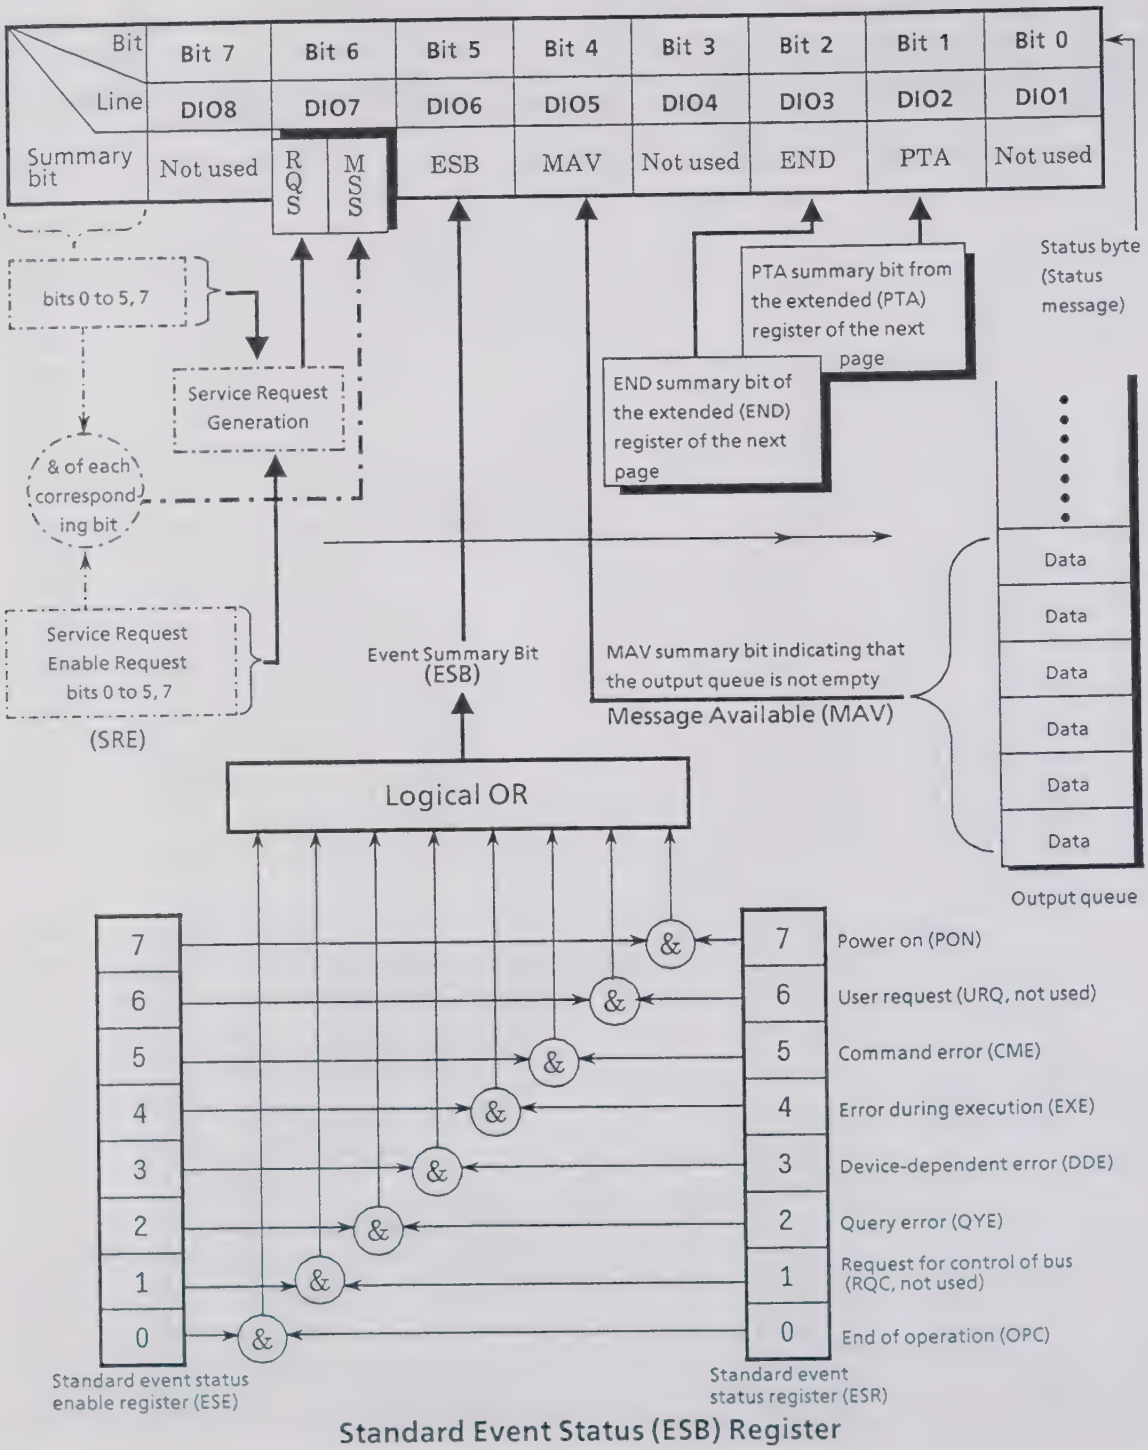

Standard Event Status (ESB) Register

Note: & indicates a conjunction (AND).

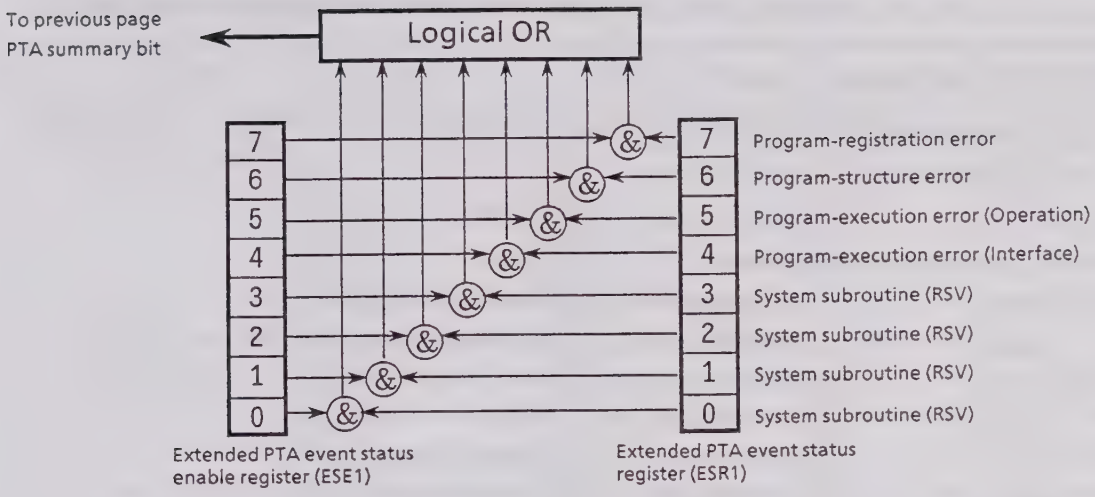

Extended PTA event status (PTA) register

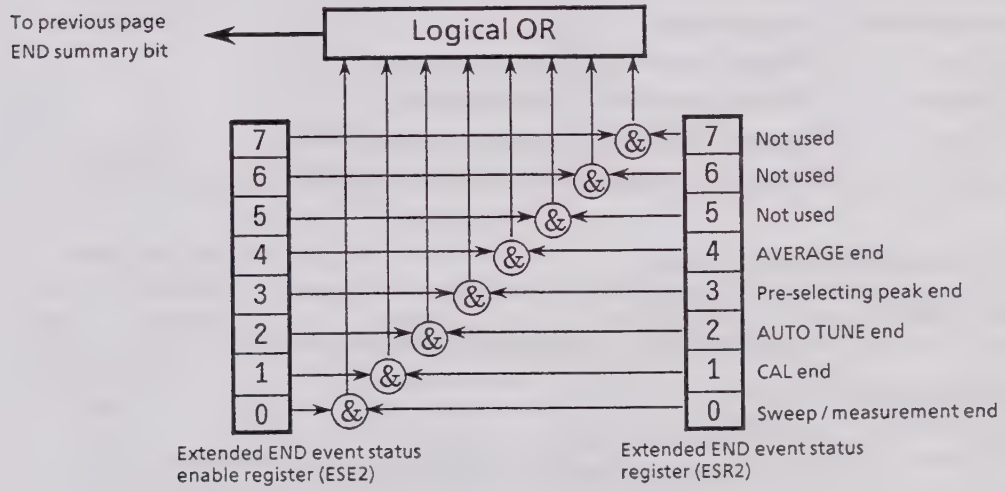

Extended END event status (END) register

(4) MS8604A device message list

MS8604A-specific program commands, query messages, and response messages are listed from the next page.

- MS8604A device message table

(a) Command messages (Command Msg)/query messages (Query Msg)

(i) Uppercase characters : Reserved words

(ii) Numeric : Reserved words (numeric code)

(iii) Lower-case characters in argument

f (frequency)	:	Real number or integer with decimal point
Units	:	GHZ, MHZ, KHZ, HZ, GZ, MZ, KZ, no units = HZ
t (time)	:	Real number or integer with decimal point
Units	:	S, SC, MS, US, no unit = MS
ℓ (level)	:	Real number or integer with decimal point
Units	:	DB, DBM, DM, DBMV, DBUV, DBUVE, V, MV, UV, W, MW, UW, NW, no units = set SCALE units
s (symbol)	:	Real number or integer with decimal point
n (no units integer)	:	Integer
r (no units real number)	:	Real number
p (position data)	:	Integer indicating a trace data position
on (On/Off switch)	:	ON/OFF or 1/0 toggle switching data
i (Data Item No.)	:	Integer indicating the number of a data items
d (Data Count)	:	Integer indicating a number of data items

(b) Response messages (Response Msg)

(i) Uppercase characters : Reserved words

(ii) Numeric : Reserved words (numeric code)

(iii) Lower-case characters in argument

f (frequency)	:	12-character fixed integer units = Hz
t (time)	:	Real number or integer with decimal point
ℓ (level)	:	Real number or integer with decimal point
u (ratio)	:	Real number or integer with decimal point
k (speed)	:	Real number or integer with decimal point
s (symbol)	:	Real number or integer with decimal point
n (no units integer)	:	Integer, variable number of digits (Significant digits are output.)
r (no units real number)	:	Real number with decimal point, variable number of digits (Significant digits are output.)
on (On/Off switch)	:	ON/OFF
a (flag)	:	Measurement result classification flag

Notes: • Integer : NR1 format, real number : NR2 format

• Ø : Zero

(a) MS8604A common command

(i) Save/Recall command

Class	Function	Item	Program Msg	Query Msg	Response Msg
Save & Recall					
	Recall from memory	Memory 1	RGRC 1	———	———
		Memory 2	RGRC 2	———	———
		Memory 3	RGRC 3	———	———
		Memory 4	RGRC 4	———	———
	Mem-Dir		RGDIR	———	———
	Recall File	file-no	RCM n	———	———
	Select Media	Int PMC	PMCS IPMC	PMCS?	IPMC
		Ext PMC1	PMCS EPMC1	PMCS?	EPMC1
		Ext PMC2	PMCS EPMC2	PMCS?	EPMC2
		Ext FD	PMCS EFD	PMCS?	EFD
	Recalled Data	Trace & Param	RDATA TP	RDATA?	TP
		Param	RDATA P	RDATA?	P
	Save to memory	Memory 1	RGSV 1	———	———
		Memory 2	RGSV 2	———	———
		Memory 3	RGSV 3	———	———
		Memory 4	RGSV 4	———	———
	Save File	file-no	SVM n		

(ii) Hard Copy command

Class	Function	Item	Program Msg	Query Msg	Response Msg
Hard Copy					
	Copy		PLS Ø	———	———
			PRINT	———	———
	⟨⟨Copy Control⟩⟩				
	Printer Type	HP2225	PMOD 3	PMOD?	PMOD 3
		ESC/P (8DOT)	PMOD 2	PMOD?	PMOD 2
		ESC/P (24DOT)	PMOD 6	PMOD?	PMOD 6
		uA455A	PMOD 5	PMOD?	PMOD 5
		MC8104A	PMOD 4	PMOD?	PMOD 4
	Printer-address	address	PRIA n	PRIA?	n

(iii) Waveform memory read command

Class	Function	Item	Program Msg	Query Msg	Response Msg
Wave Memory Data					
	Mem A	TRACE-FREQ	XMA p,b	XMA? p,d	b,b,···
	Mem B	ADJ. CH : STADARD, OCC. BW : STANDARD	XMB p,b	XMB? p,d	b,b,···
	Mem Time	TRACE-TIME	XMT p,b	XMT? p,d	b,b,···
	Mem C	Constellation	XMC pØ,p1,b	XMC? pØ,p1,d	b,b,···
	Mem D	Power measurement	XMD p,b	XMD? p,d	b,b,···
	Mem E	HIGH SPEED OCC. BW	XME p,b	XME? p,d	b,b,···
	Output Format	ASCII	BIN Ø	———	———
			BIN OFF	———	———
		BINARY	BIN 1	———	———
			BIN ON	———	———

(iv) Single/Continuous switching command

Class	Function	Item	Program Msg	Query Msg	Response Msg
Single/Continuous					
	Single		SNGLS	———	———
		Measurement/sweep end	———	SWP?	SWP Ø
		During measurement/sweep	———	SWP?	SWP 1
	Measurement / sweep sync	Single	SWP	———	———
			TS	———	———
	Continuous		CONTS		

(v) Panel mode switching command

Class	Function	Item	Program Msg	Query Msg	Response Msg
Panel Mode					
	TX Tester		PNLMD TESTER	PNLMD?	TESTER
	Spectrum		PNLMD SPECT	PNLMD?	SPECT
	System		PNLMD SYSTEM	PNLMD?	SYSTEM

(vi) System command

Class	Function	Item	Program Msg	Query Msg	Response Msg
System setup					
⟨TITLE⟩					
	User define		TITLE "·····"	TITLE?	·····
			KSE "·····"	———	———
	Display	Date/Time	TTL DATE	TTL?	DATE
		User Define	TTL USER	TTL?	USER
		off	TTL OFF	TTL?	OFF
⟨SETUP DATE/TIME⟩					
	Date		DATE yy,mm,dd	DATE?	yy,mm,dd
	Time		TIME hh,mm,ss	TIME?	hh,mm,ss
⟨HARDWARE⟩					
	RF input	HIGH	RFINPUT HIGH	RFINPUT?	HIGH
		LOW	RFINPUT LOW	RFINPUT?	LOW
	Alarm	OFF	ALARM OFF	ALARM?	OFF
			BEP Ø	———	———
			BEP OFF	———	———
		ON	ALARM ON	ALARM?	ON
			BEP 1	———	———
			BEP ON	———	———
⟨INTERFACE⟩					
	GPIB2 Address		GPIA n	GPIA?	n
	MC8104A Address		MC8104 n	MC8104?	n
	RS-232C (Option)				
	Baud rate	9600	BAUD 9600	BAUD?	9600
		4800	BAUD 4800	BAUD?	4800
		2400	BAUD 2400	BAUD?	2400
		1200	BAUD 1200	BAUD?	1200
		600	BAUD 600	BAUD?	600
		300	BAUD 300	BAUD?	300
	Parity	Even	PRTY EVEN	PRTY?	EVEN
		Odd	PRTY ODD	PRTY?	ODD
		Off	PRTY OFF	PRTY?	OFF
	Data	7Bits	DTAB 7	DTAB?	7
		8Bits	DTAB 8	DTAB?	8
	Stop Bit	1bit	STPB 1	STPB?	1
		1.5bits	STPB 1.5	STPB?	1.5
		2bits	STPB 2	STPB?	2
	Timeout		TOUT t	TOUT?	t

(vii) Other command

Class	Function	Item	Program Msg	Query Msg	Response Msg
Other					
	Display	Off	DSPL OFF	———	———
		On	DSPL ON	———	———
	Buzzer		BZR	———	———
	Terminater	LF	TRM Ø	———	———
		CR/LF	TRM 1	———	———
	Initialize		PRE	———	———
			INI	———	———
			IP	———	———
	GPIB Timeout		GTOUT t	GTOUT?	t
	Extended status	EVENT STATUS ENABLE	ESE1 n	ESE1?	n
	(PTA)	EVENT STATUS REGISTER	———	ESR1?	n
	Extended status	EVENT STATUS ENABLE	ESE2 n	ESE2?	n
	(END)	EVENT STATUS REGISTER	———	ESR2?	n

(b) TX Test mode command

(i) Screen level switching command and measurement status error information read command

Class	Function	Item	Program Msg	Query Msg	Response Msg
⟨⟨System screen switching⟩⟩					
	PDC Setup parameter		SYS PDC	SYS?	PDC
	PHS Setup parameter		SYS PHS	SYS?	PHP
	NADC Setup parameter		SYS NADC	SYS?	NADC
	Power Meter		SYS PWRMTR	SYS?	PWRMTR
⟨⟨Measurement screen switching⟩⟩					
	Modulation Analysis		MEAS MODANAL	MEAS?	MODANAL
	Constellation		MEAS CONSTEL	MEAS?	CONSTEL
	RF Power		MEAS RFPWR	MEAS?	RFPWR
	Setup Template		MEAS SETTEMP	MEAS?	SETTEMP
	Occupied Bandwidth	STD, SPECTRUM	MEAS OBW,STD	MEAS?	OBW,STD
		SPECTRUM	MEAS OBW,SPECT	MEAS?	OBW,SPECT
		HIGH SPEED	MEAS OBW,HIGH	MEAS?	OBW,HIGH
	Adjacent Channel Power	STD (ALL)	MEAS ADJ,STD1	MEAS?	ADJ,STD1
		STD (SEPARATE)	MEAS ADJ,STD2	MEAS?	ADJ,STD2
		Spect (ALL)	MEAS ADJ,SPECT1	MEAS?	ADJ,SPECT1
		Spect (SEPARATE)	MEAS ADJ,SPECT2	MEAS?	ADJ,SPECT2
		HIGH SPEED	MEAS ADJ,HIGH	MEAS?	ADJ,HIGH
	Spurious Emissions	Spot	MEAS SPURIOUS,SPOT	MEAS?	SPURIOUS,SPOT
		Search	MEAS SPURIOUS,SEARCH	MEAS?	SPURIOUS,SEARCH
	Setup Frequency Table		MEAS SETTABLE	MEAS?	SETTABLE
	Setup Sensor Cal Factor		MEAS SCALTBL	MEAS?	SCALTBL
	Back screen		BS	———	———
⟨⟨Measurement status error information read⟩⟩					
			———	MSTAT?	n

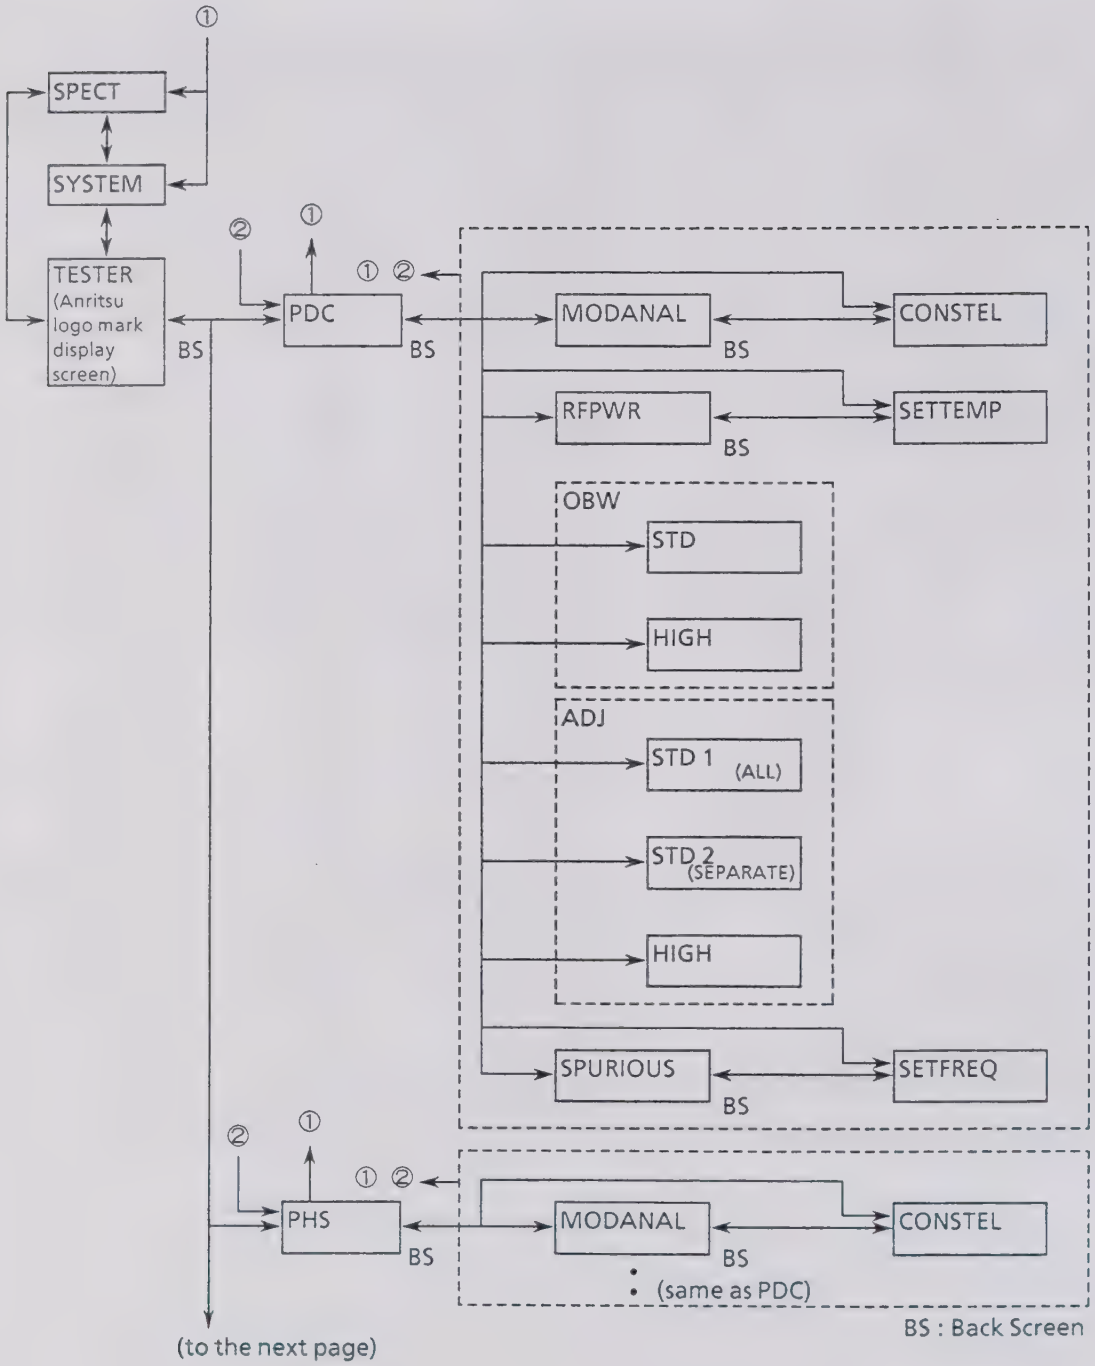

Screen level command transition (1/2)

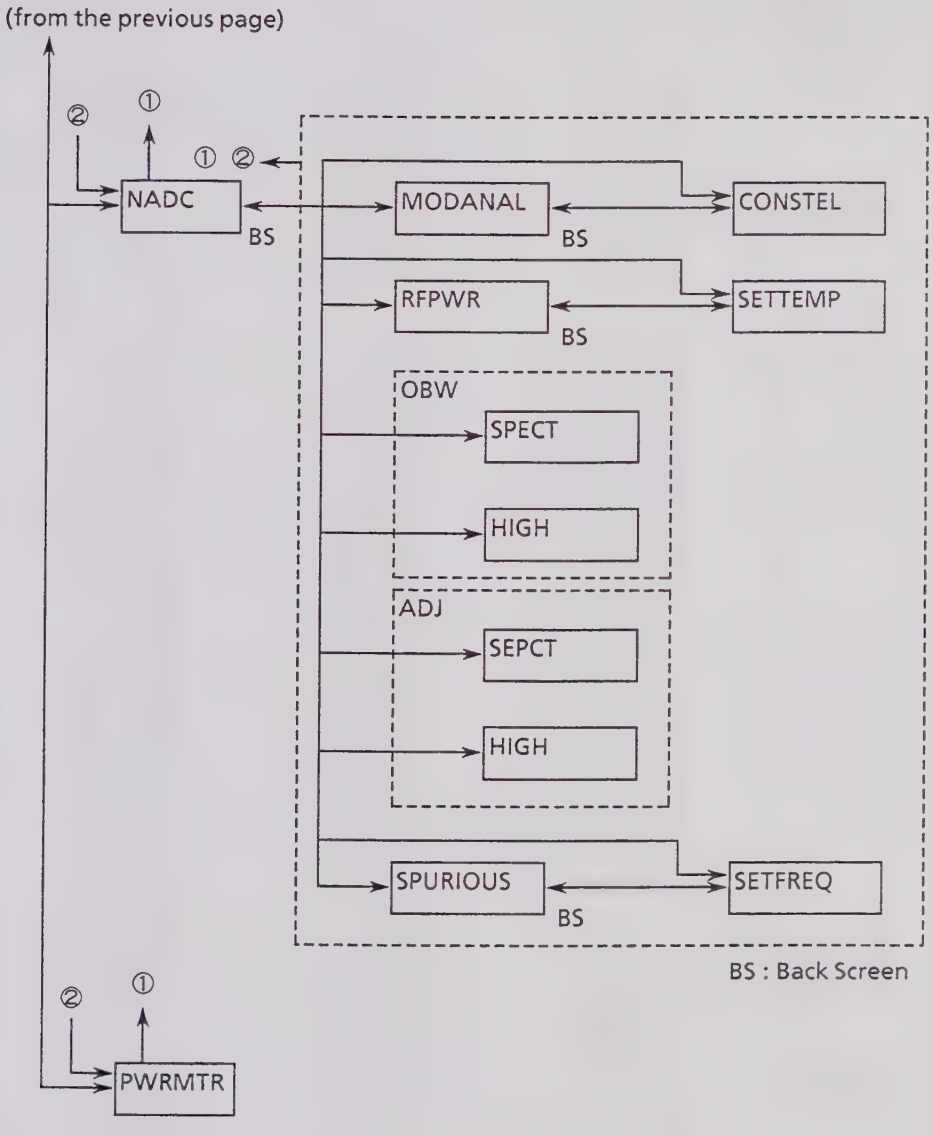

Screen level command transition (2/2)

(ii) Command at each screen

Class	Function	Item	Program Msg	Query Msg	Response Msg
Setup Parameter					
	INPUT				
	Terminal	RF	TERM RF	TERM?	RF
		I, Q-AC	TERM IQAC	TERM?	IQAC
		I, Q-DC	TERM IQDC	TERM?	IQDC
	RF level	-12 to 40	RFLVL ℓ	RFLVL?	ℓ
		Step UP	RFLVL UP	———	———
		Step DOWN	RFLVL DN	———	———
	SIGNAL				
	Measuring object	MS-CONT (PDC)	MEASOBJ MSCONT	MEASOBJ?	MSCONT
		MS-COM (PDC)	MEASOBJ MSCOM	MEASOBJ?	MSCOM
		MS-SYNC (PDC)	MEASOBJ MSSYNC	MEASOBJ?	MSSYNC
		BS-CONT (PDC)	MEASOBJ BSCONT	MEASOBJ?	BSCONT
		BS-COM (PDC)	MEASOBJ BSCOM	MEASOBJ?	BSCOM
		BS-SYNC (PDC)	MEASOBJ BSSYNC	MEASOBJ?	BSSYNC
		PS-CONT (PHS)	MEASOBJ PSCONT	MEASOBJ?	PSCONT
		PS-COM (PHS)	MEASOBJ PSCOM	MEASOBJ?	PSCOM
		CS-CONT (PHS)	MEASOBJ CSCONT	MEASOBJ?	CSCONT
		CS-COM (PHS)	MEASOBJ CSCOM	MEASOBJ?	CSCOM
		CONTINUOUS (PHS)	MEASOBJ CONT	MEASOBJ?	CONT
		MOBILE (NADC)	MEASOBJ MOBILE	MEASOBJ?	MOBILE
		SHORTENED (NADC)	MEASOBJ SHORT	MEASOBJ?	SHORT
		BASE (NADC)	MEASOBJ BASE	MEASOBJ?	BASE
	Ramp up symbol point		———	RAMPSYM?	n
	Number of symbols		———	NUMSYM?	n
	Channels per carrier	FULL RATE	CHCARR FULL	CHCARR?	FULL
		HALF RATE	CHCARR HALF	CHCARR?	HALF
	Frequency				
	Channel	1 to 9999	CHAN n	CHAN?	n
		Step UP	CHAN UP	———	———
		Step DOWN	CHAN DN	———	———
	Frequency		FREQ f	FREQ?	f
			CNF f	CNF?	CNF f
			CF f	CF?	f
		Step UP	FREQ UP	———	———
			FUP	———	———
			CF UP	———	———
		Step DOWN	FREQ DN	———	———
			FDN	———	———
			CF DN	———	———

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Setup Parameter (contd.)					
	Ch & Freq		CHFREQ n,f	———	———
		Channel (NADC)	CHNUM n	———	———
	Channel spacing		CHSPC f	CHSPC?	f
	SYNC(UNIQUE) WORD				
	Pattern	S1 (PDC)	PATT S1	PATT?	S1
		S2 (PDC)	PATT S2	PATT?	S2
		S3 (PDC)	PATT S3	PATT?	S3
		S4 (PDC)	PATT S4	PATT?	S4
		S5 (PDC)	PATT S5	PATT?	S5
		S6 (PDC)	PATT S6	PATT?	S6
		S7 (PDC)	PATT S7	PATT?	S7
		S8 (PDC)	PATT S8	PATT?	S8
		S9 (PDC)	PATT S9	PATT?	S9
		S10 (PDC)	PATT S10	PATT?	S10
		S11 (PDC)	PATT S11	PATT?	S11
		S12 (PDC)	PATT S12	PATT?	S12
		SS1 (PDC)	PATT SS1	PATT?	SS1
		SS2 (PDC)	PATT SS2	PATT?	SS2
		SS3 (PDC)	PATT SS3	PATT?	SS3
		SS4 (PDC)	PATT SS4	PATT?	SS4
		SS5 (PDC)	PATT SS5	PATT?	SS5
		SS6 (PDC)	PATT SS6	PATT?	SS6
		32 bits (PHS)	PATT B32	PATT?	B32
		16 bits (PHS)	PATT B16	PATT?	B16
		Sync1 (NADC)	PATT SYNC1	PATT?	SYNC1
		Sync2 (NADC)	PATT SYNC2	PATT?	SYNC2
		Sync3 (NADC)	PATT SYNC3	PATT?	SYNC3
		Sync4 (NADC)	PATT SYNC4	PATT?	SYNC4
		Sync5 (NADC)	PATT SYNC5	PATT?	SYNC5
		Sync6 (NADC)	PATT SYNC6	PATT?	SYNC6
		NO	PATT NO	PATT?	NO
		USER	PATT USER	PATT?	USER
			BPATT bit Bit:0···0~1···1	BPATT?	0···0~1···1
	Start point		STARTPT n	STARTPT?	n
	Transmit timing	OFF	TXTIME OFF	TXTIME?	OFF
		ON	TXTIME ON	TXTIME?	ON

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Setup Parameter (contd.)					
	Band	800 MHz	FBAND 800MHz	FBAND?	800MHz
			FBAND 800Mz	———	———
		1500 MHz	FBAND 1500MHz	FBAND?	1500MHz
			FBAND 1500Mz	———	———
	CS slot number	OFF	CSSLOT n,OFF	CSSLOT? n	OFF
		ON	CSSLOT n,ON	CSSLOT? n	ON
		active	CSNUM n	CSNUM?	n
	PS slot	OFF	PSSLOT OFF	PSSLOT?	OFF
		ON	PSSLOT ON	PSSLOT?	ON
	RCR STD-27 version	B	STD27 B	STD27?	B
		C	STD27 C	STD27?	C
	Root-Nyquist filter	Yes	RTNYQ YES	RTNYQ?	YES
			RTNYQ ON	———	———
		No	RTNYQ NO	RTNYQ?	NO
			RTNYQ OFF	———	———
	Symbol timing		SYMTIME n	SYMTIME?	n
Modulation Analysis					
	10 Burst average	On	BSTAVG ON	BSTAVG?	ON
		Off	BSTAVG OFF	BSTAVG?	OFF
	Calibration	Auto range	AUTORNG	AUTORNG?	ℓ
		Frequency adjust	FREQADJ	FREQADJ?	a,f
	Measurement result	Carrier frequency	———	CARRF?	a,f
		Carrier frequency error	———	CARRFERR?	a,f
		RMS vector error	———	VECTERR?	a,u
		First 10 symboles RMS vector error	———	FVECTERR?	a,u
		Peak vector error	———	PVECTERR?	a,u
		Magnitude error	———	MAGTDERR?	a,u
			———	MAGERR?	a,u
		Phase error	———	PHASEERR?	a,u
		Origin offset	———	ORGNOFS?	a,ℓ
		Droop factor	———	DRPFACT?	a,ℓ
		Bit rate	———	BITR?	a,k
		Bit rate error	———	BITRERR?	a,u
		Peak vector symbol	———	PVECTSYM?	a,s

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Constellation					
	Interpolation	NON-	INTPOL NON	INTPOL?	NON
		LINEAR-	INTPOL LIN	INTPOL?	LIN
		4POINT-	INTPOL POINT4	INTPOL?	POINT4
	Error scale	5%	ERRSC 5	ERRSC?	5
		10%	ERRSC 10	ERRSC?	10
		20%	ERRSC 20	ERRSC?	20
		Off	ERRSC OFF	ERRSC?	OFF
	Error scale offset	0	SCOFS 0	SCOFS?	0
		22.5	SCOFS 22.5	SCOFS?	22.5
	Calibration	Auto range	AUTORNG	AUTORNG?	ℓ
		Frequency adjust	FREQADJ	FREQADJ?	f
	Measurement result	Carrier freq error	———	CARRFERR?	a,f
		RMS vector error	———	VECTERR?	a,u
		Peak vector error	———	PVECTERR?	a,u
		Origin offset	———	ORGNOFS?	a,ℓ

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
RF Power					
	Window	Slot	WINDOW SLOT	WINDOW?	SLOT
		Frame	WINDOW FRAME	WINDOW?	FRAME
		Leading	WINDOW LEAD	WINDOW?	LEAD
			WINDOW RISE	———	———
		Trailing	WINDOW TRAIL	WINDOW?	TRAIL
			WINDOW FALL	———	———
	Marker	Normal	MKR NRM	MKR?	NRM
			MKR Ø	———	———
			M2	———	———
			MKN	———	———
		Off	MKR OFF	MKR?	OFF
			MKR 2	———	———
			MKOFF	———	———
			MKOFF ALL	———	———
			M1	———	———
	MKR position		MKP p	MKP?	p
			MKZ P	MKZ?	p
		Symbol	MKRS s	MKRS?	s
			MKZF s	MKZF?	s
			MKN s	MKN?	s
		Step UP	MKRS UP	———	———
			MKN UP	———	———
		Step DOWN	MKRS DN	———	———
			MKN DN	———	———
	MKR level		———	MKL?	ℓ
	Unit	dBm	UNIT DBM	UNIT?	DBM
			UNT Ø	UNT?	UNT Ø
			AUNITS DBM	AUNITS?	DBM
			KSA	———	———
		nW/μW/mW/W	UNIT WATT	UNIT?	WATT
			———	UNT?	UNT WATT
			———	AUNITS?	WATT
		For other screen	———	UNIT? RFPWR	DBM or WATT
	Level	Absolute	LVLREL OFF	LVLREL?	OFF
			MTEMPREL OFF	MTEMPREL?	OFF
		Relative	LVLREL ON	LVLREL?	ON
			MTEMPREL ON	MTEMPREL?	ON

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
RF Power (contd.)					
	Storage mode	Normal	STORAGE NRM	STORAGE?	NRM
		Max hold	STORAGE MAX	STORAGE?	MAX
		Min hold	STORAGE MIN	STORAGE?	MIN
		Average			
		ON	STORAGE AVG	STORAGE?	AVG
			VAVG ON	———	———
			VAVG 1	———	———
			KSG	———	———
		OFF	VAVG OFF	———	———
			VAVG 0	———	———
			KSH	———	———
		Cumulative	STORAGE CUM	STORAGE?	CUM
		Over write	STORAGE OVER	STORAGE?	OVER
		Wide dynamic range	STORAGE WIDE	STORAGE?	WIDE
		For other screen	———	STORAGE? RFPWR	NRM MAX MIN AVG CUM OVER WIDE
	Average No.	2 to 99	AVR n	AVR?	n
			VAVG n	VAVG?	n
		For other screen	———	AVR? RFPWR	n
	Calibration	(See Modulation Analysis)			
	Select template	No.1	SLCTTEMP NO1	SLCTTEMP?	NO1
		No.2	SLCTTEMP NO2	SLCTTEMP?	NO2
		No.3	SLCTTEMP NO3	SLCTTEMP?	NO3
		Standard	SLCTTEMP STD	SLCTTEMP?	STD
		Off	SLCTTEMP OFF	SLCTTEMP?	OFF
		Not selected	———	SLCTTEMP?	NOT
	Measurement result	TX power	———	TXPWR?	a,ℓ depends on display units
			———	TXPWR? DBM	a,ℓ
			———	TXPWR? WATT	a,ℓ
		Carrier OFF power	———	OFFPWR?	a,ℓ depends on display units
			———	OFFPWR? DBM	a,ℓ
				OFFPWR? WATT	a,ℓ
		ON/OFF ratio	———	RATIO?	a,u

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
RF Power (contd.)					
	Measurement result (contd.)	Modulation power	———	HMODPWR?	a,ℓ depends on display units
			———	HMODPWR? DBM	a,ℓ
			———	HMODPWR? WATT	a,ℓ
		Timing	———	TIMING?	a,s
		Jitter (+)	———	JITTER? +	a,s
		Jitter (−)	———	JITTER? −	a,s
		Slot MOD power	———	SLOTPWER? n	a,ℓ
Setup template					
	Save template	No.1	SAVETEMP NO1	———	NO1
		No.2	SAVETEMP NO2	———	NO2
		No.3	SAVETEMP NO3	———	NO3
	Level Modify	Limit-1	TEMPLVL 1,ℓ	TEMPLVL? 1	ℓ
		Limit-2	TEMPLVL 2,ℓ	TEMPLVL? 2	ℓ
		Limit-3	TEMPLVL 3,ℓ	TEMPLVL? 3	ℓ
		Limit-4	TEMPLVL 4,ℓ	TEMPLVL? 4	ℓ
		Limit-5	TEMPLVL 5,ℓ	TEMPLVL? 5	ℓ
Occupied Bandwidth					
	Method	STD, SPECTRUM	MEAS OBW,STD	MEAS?	OBW,STD
		SPECTRUM	MEAS OBW,SPECT	MEAS?	OBW,SPECT
		HIGH SPEED	MEAS OBW,HIGH	MEAS?	OBW,HIGH
	Storage mode	(See RF power : Normal and Average)			
		For other screen	———	STORAGE? OBW	NRM AVG
	Average No.	(See RF power)			
		For other screen	———	AVR? OBW	n
	Calibration	(See Modulation Analysis)			
	Measurement result	Occ. BW	———	OCCBW?	a,f
			———	OBW?	a,f
		CENTER	———	OBWFREQ? CENTER	a,f
		LOWER	———	OBWFREQ? LOWER	a,f
			———	OBWFREQ? −	a,f
		UPPER	———	OBWFREQ? UPPER	a,f
			———	OBWFREQ? +	a,f

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Adjacent Chanel Power					
	Method	STD (ALL)	MEAS ADJ,STD1	MEAS?	ADJ,STD1
		STD (SEPARATE)	MEAS ADJ,STD2	MEAS?	ADJ,STD2
		Spect (ALL)	MEAS ADJ,SPECT1	MEAS?	ADJ,SPECT1
		Spect (SEPARATE)	MEAS ADJ,SPECT2	MEAS?	ADJ,SPECT2
		HIGH SPEED	MEAS ADJ,HIGH	MEAS?	ADJ,HIGH
	Unit	dBm	UNIT DBM	UNIT?	DBM
			UNT Ø	UNT?	UNT Ø
			AUNITS DBM	AUNITS?	DBM
			KSA	———	———
		mW	UNIT MW	UNIT?	MW
			———	UNT?	UNT MW
			———	AUNITS?	MW
		μW	UNIT UW	UNIT?	UW
			———	UNT?	UNT UW
			———	AUNITS?	UW
		nW	UNIT NW	UNIT?	NW
			———	UNT?	UNT NW
			———	AUNITS?	NW
		dB	UNIT DB	UNIT?	DB
			———	UNT?	UNT DB
			———	AUNITS?	DB
		For other screen	———	UNIT? ADJ	DBM MW UW NW DB
	Storage mode	(See RF power)			
		For other screen	———	STORAGE?ADJ	NRM AVG
	Average No.	(See Occupied Bandwidth)			
		For other screen	———	AVR? ADJ	n
	Calibration	(See Modulation Analysis)			
	Marker	OFF	ADJMEAS OFF	ADJMEAS?	OFF
		ON	ADJMEAS ON	ADJMEAS?	ON

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Adjacent Chanel Power (contd.)					
	MKR position		MKP p	MKP?	p
			MKZ p	MKP?	p
		Frequency	MKRS f	MKRS?	f
			MKZF f	MKZF?	f
			MKN f	MKN?	f
		step UP	MKRS UP	———	———
			MKN UP	———	———
		step DOWN	MKRS DN	———	———
			MKN DN	———	———
	MKR level		———	MKL?	ℓ
	Measurement result	Lower-3	———	ADJCH? LOW3	a,ℓ
		Lower-2	———	ADJCH? LOW2	a,ℓ
		Lower-1	———	ADJCH? LOW1	a,ℓ
		Upper-1	———	ADJCH? UP1	a,ℓ
		Upper-2	———	ADJCH? UP2	a,ℓ
		Upper-3	———	ADJCH? UP3	a,ℓ
			———	ADJCH? ps,un	a,ℓ
	Peak Power (HIGH)	Lower-3 to Upper-3	———	PEAKPWR? ps	a,ℓ depends on display units.
	Peak Power from Switching Transients (HIGH)		———	PEAKPWR? ps,un	a,ℓ
	Mean Power (HIGH)	Lower-2 to Upper-2	———	MEANPWR? ps	a,ℓ depends on display units.
			———	MEANPWR? ps,un	a,ℓ
	Mean Power due to Modulation (HIGH)	Lower-3 to Upper-3	———	MODPWR? ps	a,ℓ depends on display units.
			———	MODPWR? ps,un	a,ℓ
	Peak Power from Switching Transients (HIGH)	Lower-3	———	SWPWR? ps	a,ℓ depends on display units.
		Upper-3	———	SWPWR? ps,un	a,ℓ
			ps:LOW3,LOW2,LOW1,UP1,UP2,UP3 un:DBM,WATT,DB		

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Spurious Emissions					
	Select frequency table	No.1	SLCTTBL NO1	SLCTTBL?	NO1
		No.2	SLCTTBL NO2	SLCTTBL?	NO2
		No.3	SLCTTBL NO3	SLCTTBL?	NO3
		Not selected	———	SLCTTBL?	NOT
	Unit	(See Adjacent CH Power)			
		For other screen	———	UNIT? SPURIOUS	DBM MW UW NW DB
	Calibration	(See Modulation Analysis)			
	RF Attenuation	Normal	RFATTN NRM	RFATTN?	NRM
		Noise	RFATTN NOISE	RFATTN?	NOISE
	Measurement result	f1 to f15	———	SPULVL? fn	a,ℓ depends on display units.
			———	SPULVL? fn,un	a,ℓ
			fn:F1 to F15,un:DBM,WATT,DB		
	Spurious mode	SPOT	MEAS SPURIOUS,SPOT	MEAS?	SPURIOUS,SPOT
		SEARCH	MEAS SPURIOUS,SEARCH	MEAS?	SPURIOUS,SEARCH
Setup Frequency Table					
	Save frequency table	No.1	SAVETBL NO1	———	———
		No.2	SAVETBL NO2	———	———
		No.3	SAVETBL NO3	———	———
	Frequency Modify	f1	SPUFREQ F1,f	SPUFREQ? F1	f
		f2	SPUFREQ F2,f	SPUFREQ? F2	f
		f3	SPUFREQ F3,f	SPUFREQ? F3	f
		f4	SPUFREQ F4,f	SPUFREQ? F4	f
		F5	SPUFREQ F5,f	SPUFREQ? F5	f
		f6	SPUFREQ F6,f	SPUFREQ? F6	f
		f7	SPUFREQ F7,f	SPUFREQ? F7	f
		f8	SPUFREQ F8,f	SPUFREQ? F8	f
		f9	SPUFREQ F9,f	SPUFREQ? F9	f
		f10	SPUFREQ F10,f	SPUFREQ? F10	f
		f11	SPUFREQ F11,f	SPUFREQ? F11	f
		f12	SPUFREQ F12,f	SPUFREQ? F12	f
		f13	SPUFREQ F13,f	SPUFREQ? F13	f
		f14	SPUFREQ F14,f	SPUFREQ? F14	f
		f15	SPUFREQ F15,f	SPUFREQ? F15	f
		Cancel	SPUFREQ fn,0 (fn:F1 to F15)	———	———
		Harmonics	SPUFREQ HRM	———	———
			SPUHARM	———	———

(ii) Command at each screen (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Power Meter					
	Frequency		FREQ f	FREQ?	f
			CNF f	CNF?	CNF f
			CF f	CF?	f
		Step UP	FREQ UP	———	———
			FUP	———	———
			CF UP	———	———
		Step DOWN	FREQ DN	———	———
			FDN	———	———
			CF DN	———	———
		For other screen	———	FREQ? PWRMTR	f
	Set relative		SETREL	———	———
			DBR	———	———
	Sensor connect to	Tester	SCNCT TESTER	SCNCT?	TESTER
		DUT	SCNCT DUT	SCNCT?	DUT
	Cal factor	Sensor	———	CSCAL?	ℓ
		User	UCAL ℓ	UCAL?	ℓ
			OFF ℓ	———	———
		Reference	———	CRCAL?	ℓ
	Cal oscillator	On	CALOSC ON	CALOSC?	ON
			COS	———	———
		Off	CALOSC OFF	CALOSC?	OFF
			CST	———	———
	Cal adjust		CALADJ	———	———
			CDJ	———	———
	Zero set		ZEROSET	———	———
			ZAJ	———	———
	Range	Auto	RNG AUTO	RNG?	AUTO
			RNGA	———	———
		Hold	RNG HOLD	RNG?	HOLD
		Hold (0.1 mW)	RNG2	———	———
		Hold (1 mW)	RNG3	———	———
		Hold (10 mW)	RNG4	———	———
		Hold (100 mW)	RNG5	———	———
	Measurement result	Power	———	POWER? DBM	ℓ
			———	POWER? WATT	ℓ
			———	POWER? DB	ℓ
Setup Sensor Cal Factor					
	Cal Factor		SCALT f,ℓ	SCALT? f	ℓ

(c) Spectrum mode command

Class	Function	Item	Program Msg	Query Msg	Response Msg
Signal Search					
	Auto Tune		ATUN	———	———
	Peak to CF		PCF	———	———
	Peak to REF		PRL	———	———
Freq/Amplitude					
	<<Frequency>>				
	Freq Mode	Center-Span	FRQ Ø	FRQ?	FRQ Ø
		Start-Span	FRQ 1	FRQ?	FRQ 1
		Start-Stop	FRQ 2	FRQ?	FRQ 2
	Center Freq		CNF f	CNF?	CNF f
			CF f	CF?	f
	Freq step UP		FUP	———	———
			CF UP	———	———
	Freq step DOWN		FDN	———	———
			CF DN	———	———
	Start Freq		STF f	STF?	STF f
			FA f	FA?	f
	Stop Freq		SOF f	SOF?	SOF f
			FB f	FB?	f
	Freq Step Size		FSS f	FSS?	FSS f
			SS f	SS?	f
	<<Span>>				
	Freq Span		SPF f	SPF?	SPF f
			SP f	SP?	f
	Freq-Span step UP		SPU	———	———
			SP UP	———	———
	Freq-Span step DOWN		SPD	———	———
			SP DN	———	———
	Full Span		FS	———	———
	Zero Span		SPF Ø	———	———
	Band Select	Auto : 0 Hz to 8.5 GHz	BNDC AUTO	BNDC?	AUTO
			HNLOCK OFF	HNLOCK?	OFF
			HNUNLK	———	———

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Freq/Amplitude (contd.)					
	Band Select (contd.)	Band 0 : 0 Hz to 2 GHz	BNDC Ø	BNDC?	Ø
			HNLOCK Ø	HNLOCK?	ON
			HN Ø	HN?	Ø
		Band 1 − : 1.7 to 8.5 GHz	BNDC 1-	BNDC?	1-
			HNLOCK 1	HNLOCK ?	ON
			HN 1	HN?	1
		Band 1 + : 6.5 to 8.5 GHz	BNDC 1+	BNDC?	1+
			HNLOCK 2	HNLOCK?	ON
			HN 2	HN?	2
	<<Amplitude>>				
	REF Level		RLV ℓ	RLV?	RLV ℓ
			RL ℓ	RL?	ℓ
	REF-level step UP		RL UP	———	———
	REF-level step DOWN		RL DN	———	———
	Log Scale Step Size	Manual	LSS ℓ	LSS?	LSS ℓ
		AUTO : 1 div	LSSA 1	LSSA?	LSSA 1
		2 div	LSSA 2	LSSA?	LSSA 2
		5 div	LSSA 5	LSSA?	LSSA 5
		10 div	LSSA 1Ø	LSSA?	LSSA 1Ø
	Log Scale Range	1 dB/Div	SCL Ø	SCL?	SCL Ø
			LG 1DB	LG?	1
		2 dB/Div	SCL 1	SCL?	SCL 1
			LG 2DB	LG?	2
		5 dB/Div	SCL 2	SCL?	SCL 2
			LG 5DB	LG?	5
		10 dB/Div	SCL 3	SCL?	SCL 3
			LG 1ØDB	LG?	1Ø
		Scale UP	LG UP	———	———
		Scale DOWN	LG DN	———	———
	Linear Scale Range	Lin scale	LN	———	———
			LG Ø	———	———
		1 %/Div	SCL 4	SCL?	SCL 4
		2 %/Div	SCL 5	SCL?	SCL 5
		5 %/Div	SCL 6	SCL?	SCL 6
		10 %/Div	SCL 7	SCL?	SCL 7

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
	Log Unit	dBm	UNT Ø	UNT?	UNT Ø
			AUNITS DBM	AUNITS?	DBM
			KSA	———	———
		dBμV	UNT 1	UNT?	UNT 1
			AUNITS DBUV	AUNITS?	DBUV
			KSC	———	———
		dBmV	UNT 2	UNT?	UNT 2
			AUNITS DBMV	AUNITS?	DBMV
			KSB	———	———
		V	UNT 3	UNT?	UNT 3
			AUNITS V	AUNITS?	V
			KSD	———	———
		dBμV (emf)	UNT 4	UNT?	UNT 4
			AUNITS DBUVE	AUNTIS?	DBUVE
Sweep Control					
	Zone Sweep	Off	PSW Ø	———	———
			PSW OFF	PSW?	PSW OFF
		On	PSW 1	———	———
			PSW ON	PSW?	PSW?
	Tracking	Off	MKTRACK Ø	———	———
			MKTRACK OFF	MKTRACK?	OFF
			MT Ø	———	———
		On	MKTRACK 1	———	———
			MKTRACK ON	MKTRACK?	ON
			MT1	———	———
	Gate	Off	GATE Ø	———	———
			GATE OFF	GATE?	OFF
		On	GATE 1	———	———
			GATE ON	GATE?	ON
	Gate Delay		GD t	GD?	t
	Gate Length		GL t	GL?	t
	Gate End	Int	GE INT	GE?	INT
		Ext	GE EXT	GE?	EXT
	Trigger SW	Freerun	TRGS FREE	TRGS?	FREE
		Triggered	TRGS TRGD	TRGS?	TRGD

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Sweep Control (contd.)					
	Trigger Mode	Freerun	TRG Ø	TRG?	TRG Ø
			TM FREE	TM?	FREE
		Video	TRG 1	TRG?	TRG 1
			TM VID	TM?	VID
		Line	TRG 2	TRG?	TRG 2
			TM LINE	TM?	LINE
		Ext	TRG 3	TRG?	TRG 3
			TM EXT	TM?	EXT
		TV	TRG 6	TRG?	TRG 6
			TM TV	TM?	TV
	Trigger Sourece	Video	TRGSOURCE VID	TRGSOURCE?	VID
		Line	TRGSOURCE LINE	TRGSOURCE?	LINE
		Ext	TRGSOURCE EXT	TRGSOURCE?	EXT
		TV	TRGSOURCE TV	TRGSOURCE?	TV
	Ext Trigger Type	Input 1 (±10 V)	EXTTYPE 10V	EXTTYPE?	10V
		Input 2 (TTL)	EXTTYPE TTL	EXTTYPE?	TTL
	TV Type	PAL	TVSTND PAL	TVSTND?	PAL
		NTSC	TVSTND NTSC	TVSTND?	NTSC
	TV-Sync	V-sync	TVSFRM VERTICAL	TVSFRM?	VERTICAL
		H-sync (even)	TVSFRM EVEN	TVSFRM?	EVEN
		H-sync (odd)	TVSFRM ODD	TVSFRM?	ODD
	TV (H-Sync line)		TVLINE n	TVLINE?	n
	Trigger Level		TRGLVL r	TRGLVL?	r
	Trigger Slope	Rise	TRGSLP RISE	TRGSLP?	RISE
		Fall	TRGSLP FALL	TRGSLP?	FALL
(Read/Write SW)					
	Trace-Freq Write Switch	View	AWR Ø	———	———
			AWR OFF	AWR?	AWR OFF
			VIEW TRA	———	———
		Write	AWR 1	———	———
			AWR ON	AWR?	AWR ON
			CLRW TRA	———	———
			A1	———	———
	Trace-Time Write Switch	View	TMWR Ø	———	———
			TMWR OFF	TMWR?	TMWR OFF
			VIEW TRTIME	———	———
		Write	TMWR 1	———	———
			TMWR ON	TMWR?	TMWR ON
			CLRW TRTIME	———	———

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Coupled Function (RBW/VBW/SWT/ATTEN)					
	RBW	Manual	ARB Ø	ARB?	ARB Ø
		Auto	ARB 1	ARB?	ARB 1
			RB AUTO	———	———
			CR	———	———
	RBW (Manual)	10 Hz	RB 10HZ	RB?	10
			RBW 13	RBW?	RBW 13
		30 Hz	RB 30HZ	RB?	30
			RBW Ø	RBW?	RBW Ø
		100 Hz	RB 100HZ	RB?	100
			RBW 1	RBW?	RBW 1
		300 Hz	RB 300HZ	RB?	300
			RBW 2	RBW?	RBW 2
		1 kHz	RB 1KHZ	RB?	1000
			RBW 3	RBW?	RBW 3
		3 kHz	RB 3KHZ	RB?	3000
			RBW 4	RBW?	RBW 4
		10 kHz	RB 10KHZ	RB?	10000
			RBW 5	RBW?	RBW 5
		30 kHz	RB 30KHZ	RB?	30000
			RBW 6	RBW?	RBW 6
		100 kHz	RB 100KHZ	RB?	100000
			RBW 7	RBW?	RBW 7
		300 kHz	RB 300KHZ	RB?	300000
			RBW 8	RBW?	RBW 8
		1 MHz	RB 1MHZ	RB?	1000000
			RBW 9	RBW?	RBW 9
		3 MHz	RB 3MHZ	RB?	3000000
			RBW 14	RBW?	RBW 14
		Step UP	RB UP	———	———
		Step DOWN	RB DN	———	———
	VBW	Manual	AVB Ø	AVB?	AVB Ø
		AUTO	AVB 1	AVB?	AVB 1
			VB AUTO	———	———
			CV	———	———

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Coupled Function (RBW/VBW/SWT/ATTEN) (contd.)					
	VBW (Manual)	1 Hz	VB 1HZ	VB?	1
			VBW 0	VBW?	VBW 0
		3 Hz	VB 3HZ	VB?	3
			VBW 8	VBW?	VBW 8
		10 Hz	VB 10HZ	VB?	10
			VBW 1	VBW?	VBW 1
		30 Hz	VB 30HZ	VB?	30
			VBW 9	VBW?	VBW 9
		100 Hz	VB 100HZ	VB?	100
			VBW 2	VBW?	VBW 2
		300 Hz	VB 300HZ	VB?	300
			VBW 10	VBW?	VBW 10
		1 kHz	VB 1KHZ	VB?	1000
			VBW 3	VBW?	VBW 3
		3 kHz	VB 3KHZ	VB?	3000
			VBW 11	VBW?	VBW 11
		10 kHz	VB 10KHZ	VB?	10000
			VBW 4	VBW?	VBW 4
		30 kHz	VB 30KHZ	VB?	30000
			VBW 12	VBW?	VBW 12
		100 kHz	VB 100KHZ	VB?	100000
			VBW 5	VBW?	VBW 5
		300 kHz	VB 300KHZ	VB?	300000
			VBW 13	VBW?	VBW 13
		1 MHz	VB 1MHZ	VB?	1000000
			VBW 7	VBW?	VBW 7
		3 MHz	VB 3MHZ	VB?	3000000
			VBW 14	VBW?	VBW 14
		Off	VB OFF	VB?	OFF
			VBW 6	VBW?	VBW 6
			AVB 2	AVB?	AVB 2
		Step UP	VB UP	———	———
		Step DOWN	VB DN	———	———
	VBW/RBW ratio	Ratio	VBR r	VBR?	r
	SWT	Manual	AST 0	AST?	AST 0
		AUTO	AST 1	AST?	AST 1
			ST AUTO	———	———
			CT	———	———

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Coupled Function (RBW/VBW/SWT/ATTEN) (contd.)					
	SWT (Manual)	Time	SWT t	SWT?	SWT t
			ST t	ST?	t
		Step UP	ST UP	———	———
		Step DOWN	ST DN	———	———
	ATTEN	Manual	AAT Ø	AAT?	AAT Ø
		Auto	AAT 1	AAT?	AAT 1
			AT AUTO	———	———
			CA	———	———
	ATTEN (Manual)	0 to 11	ATT n	ATT?	ATT n
		0 dB	AT Ø	AT?	Ø
		5 dB	AT 5	AT?	5
		10 dB	AT 10	AT?	10
		15 B	AT 15	AT?	15
		20 dB	AT 20	AT?	20
		25 dB	AT 25	AT?	25
		30 dB	AT 30	AT?	30
		35 dB	AT 35	AT?	35
		40 dB	AT 40	AT?	40
		45 dB	AT 45	AT?	45
		50 dB	AT 50	AT?	50
		55 dB	AT 55	AT?	55
		60 dB	AT 60	AT?	60
		65 dB	AT 65	AT?	65
		70 dB	AT 70	AT?	70
		75 dB	AT 75	AT?	75
		Step UP	AT UP	———	———
		Step DOWN	AT DN	———	———
	BW/SWT Auto		BSAUTO	———	———
	ALL Auto		AUTO	———	———

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Marker					
	Marker Mode	Normal	MKR Ø	MKR?	MKR Ø
			M2	———	———
		Delta	MKR 1	MKR?	MKR 1
			MKD	———	———
			M3	———	———
		Off	MKR 2	MKR?	MKR 2
			MKOFF	———	———
			MKOFF ALL	———	———
			M1	———	———
	Zone Center	Position	MKZ p	MKZ?	MKZ p
			MKP p	MKP?	p
		Freq set	MKZF f	MKZF?	f
			MKN f	MKN?	f
		Time set	MKZF t	MKZF?	t
			MKN t	MKN?	t
		Step UP	MKN UP	———	———
		Step DOWN	MKN DN	———	———
	Zone Width	Frequency	MZWF f	MZWF?	f
		Points	MZW p	MZW?	MZW p
		Spot	MKW 1	MKW?	MKW 1
		1 div	MKW 5	MKW?	MKW 5
		2 div	MKW 6	MKW?	MKW 6
		5 div	MKW 7	MKW?	MKW 7
		10 div	MKW 2	MKW?	MKW 2
	<<Marker Func>>				
	MKR to CF		MKR 3	———	———
			MKCF	———	———
			E2	———	———
	MKR to REF		MKR 4	———	———
			MKRL	———	———
			E4	———	———
	MKR to CFstep		MKR 5	———	———
			MKSS	———	———
			E3	———	———
	△MKR to Span		MKR 6	———	———
			MKSP	———	———
			KSO	———	———
	Zone to Span		MKR 7	———	———

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Marker (contd.)					
	<<Multi Marker>>				
	Multi Marker	Off	MKMULTI Ø	———	———
			MKMULTI OFF	MKMULTI?	OFF
		On	MKMULTI 1	———	———
			MKMULTI ON	MKMULTI?	ON
	Multi Marker (Highest 10)		MKMHI	———	———
	Multi Marker (Harmonics)		MKMHRM	———	———
	Multi Marker	Off	MKSLCT n,Ø	———	———
			MKSLCT n,OFF	MKSLCT? n	OFF
		On	MKSLCT n,1	———	———
			MKSLCT n,ON	MKSLCT? n	ON
	Select Active Marker	1 to 10	MKACT n	MKACT?	n
	Setup Marker Position	1 to 10, f	MKMP n,f	MKMP? n	f
	Clear Multi Marker		MKMCL	———	———
	Multi Marker List	Off	MKLIST Ø		
			MKLIST OFF	MKLIST?	OFF
		On	MKLIST 1		
			MKLIST ON	MKLIST?	ON
	Multi Marker List Query (Level)		———	MKML? n	ℓ
	<<Peak Search>>				
	Peak		MKS Ø	———	———
			MKPK	———	———
			MKPK HI	———	———
			E1	———	———
	Next Peak		MKS 1	———	———
			MKPK NH	———	———
	Min Dip		MKS 2	———	———
			MKMIN	———	———
	Next Right Peak		MKS 9	———	———
			MKPK NR	———	———
	Next Left Peak		MKS 1Ø	———	———
			MKPK NL	———	———
	Next Dip		MKS 11	———	———

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Marker (contd.)					
	<<Input Position>>				
	Reference Marker (query)		———	RMK?	RMK p
	Current Marker (query)		———	CMK?	CMK p
	Marker Pos (query)	Freq	———	MKF?	f
		Time	———	MKF?	t
		Level	———	MKL?	ℓ
			———	MKA?	ℓ
		FM : freq	———	MKL?	f
			———	MKA?	f
		EXT TRIG : time	———	MKL?	t
			———	MKA?	t
Display					
	<<Display Mode>>				
	A (FREQ)		DFMT A	DFMT?	A
	Time		DFMT TIME	DFMT?	TIME
	<<Storage Mode>>				
	Normal	A (FREQ)	AMD Ø	AMD?	AMD Ø
		Time	TMMD Ø	TMMD?	TMMD Ø
	Max hold	A	AMD 1	AMD?	AMD 1
			MXMH TRA	———	———
			A2	———	———
		Time	TMMD 1	TMMD?	TMMD 1
	Min hold	A	AMD 3	AMD?	AMD3
		Time	TMMD 3	TMMD?	TMMD 3
	Average	A	AMD 2	AMD?	AMD 2
		Time	TMMD 2	TMMD?	TMMD 2
		Off	VAVG Ø	———	———
			VAVG OFF	———	———
			KSH	———	———
		On	VAVG 1	———	———
			VAVG ON	———	———
			KSG	———	———
	Cumulative	A	AMD 4	AMD?	AMD 4
		Time	TMMD 4	TMMD?	TMMD 4
	Over write	A	AMD 5	AMD?	AMD 5
		Time	TMMD 5	TMMD?	TMMD 5
	View	A	VIEW TRA	———	———
		Time	VIEW TRTIME	———	———

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Display (contd.)					
	Average count	2	VAVG 2	VAVG?	2
		4	AVR Ø	AVR?	AVR Ø
			VAVG 4	VAVG?	4
		8	AVR 1	AVR?	AVR 1
			VAVG 8	VAVG?	8
		16	AVR 2	AVR?	AVR 2
			VAVG 16	VAVG?	16
		32	AVR 3	AVR?	AVR 3
			VAVG 32	VAVG?	32
		64	VAVG 64	VAVG?	64
		128	AVR 4	AVR?	AVR 4
			VAVG 128	VAVG?	128
		256	VAVG 256	VAVG?	256
	Det mode (A)	Positive Peak	DETM TRA,POS	DETM? TRA	POS
		Sample	DETM TRA,SMP	DETM? TRA	SMP
		Negative peak	DETM TRA,NEG	DETM? TRA	NEG
	<<time>>				
	Time Delay	t	TDLY t	TDLY?	t
	Time Span	t	TSP t	TSP?	t
	Zone (expand mode)	Off	TZONE Ø	———	———
			TZONE OFF	TZONE?	OFF
		On	TZONE 1	———	———
			TZONE ON	TZONE?	ON
	Expand mode	Off	TEXPAND Ø		
			TEXPAND OFF	TEXPAND?	OFF
		On	TEXPAND 1		
			TEXPAND ON	TEXPAND?	ON
	Zone Start	t	TZSTART t	TZSTART?	t
	Zone Span	t	TZSP t	TZSP?	t
	Special Function (FM/TRIG MONITOR)	FM	SPFUNC FM	SPFUNC?	FM
		Ext Trigger Monitor	SPFUNC EXT	SPFUNC?	EXT
		Off	SPFUNC OFF	SPFUNC?	OFF
	FM Range	200 kHz/div	FMRNG 200KHZ	FMRNG?	200000
		20 kHz/div	FMRNG 20KHZ	FMRNG?	20000
		2 kHz/div	FMRNG 2KHZ	FMRNG?	2000
	Coupling (FM)	AC	COUPLE AC	COUPLE?	AC
		DC	COUPLE DC	COUPLE?	DC

(c) Spectrum mode command (contd.)

Class	Function	Item	Program Msg	Query Msg	Response Msg
Sound					
	Monitor	AM	MON AM	MON?	AM
		FM	MON FM	MON?	FM
		Off	MON OFF	MON?	OFF
	Monitor Volume	n	MONVOL n	MONVOL?	n
Parameter					
	Parameter	Page 1	PARAM 1	PARAM?	1
		Page 2	PARAM 2	PARAM?	2
		Off	PARAM OFF	PARAM?	OFF
System					
	Auto Sweep Time	Fast	ASWT FAST	ASWT?	FAST
		Slow	ASWT SLOW	ASWT?	SLOW
	Data Point	Normal	DPOINT NRM	DPOINT?	NRM
		Double	DPOINT DOUBLE	DPOINT?	DOUBLE
	Couple Mode	Common	VBCOUPLE COM	VBCOUPLE?	COM
		Independent	VBCOUPLE IND	VBCOUPLE?	IND
Calibration					
	All		CAL Ø	———	———
	Freq		CAL 1	———	———
	Level		CAL 2	———	———
	Preselector Tune	Auto tune	PRESEL AUTO	PRESEL?	AUTO
			PP	———	———
		Manual tune	PRESEL n	PRESEL?	n
		Preset	PRESEL PRESET	PRESEL?	PRESET
Cal/Uncal					
	Uncal display	Off	UNC Ø	———	———
			UNC OFF	UNC?	UNC OFF
		On	UNC 1	———	———
			UNC ON	UNC?	UNC ON
	Uncal status	Normal	———	UCL?	UCL Ø
		Uncal	———	UCL?	UCL 1

SECTION 2
CONNECTING THE BUS AND SETTING THE ADDRESS

This section describes how to connect the GPIB cable and set the addresses in order to set-up the system before using the GPIB.

TABLE OF CONTENTS

2.1 Connecting Devices with GPIB Cables 2-3

2.2 Setting and Checking GPIB addresses 2-4

(Blank)

2.1 Connecting Devices with GPIB Cables

The rear panel has connectors for connecting GPIB cables.

A maximum of 15 devices, including the controller, can be connected to one system. The restrictions indicated at the right of the diagram below should be observed when connecting many devices to one system.

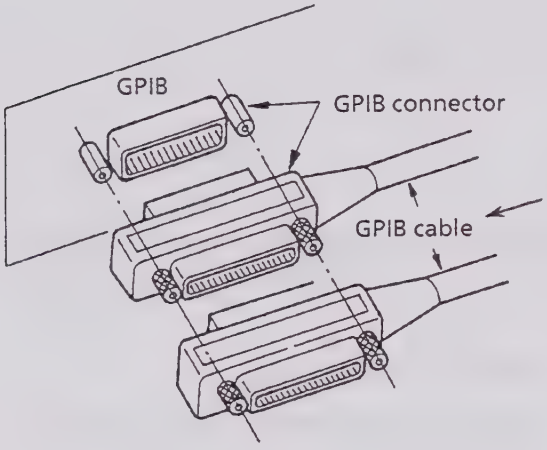

Total cable length	≦ 20 m
Each cable length between devices	≦ 4 m
Number of devices which can be connected	≦ 15

CAUTION

The cables must be connected before the power is switched on.

2.2 Setting and Checking GPIB addresses

Initial values of GPIB addresses are as follows:

GPIB1 address : 1
GPIB2 address : 16
MC8104A address : 19
Printer address : 17

Change these addresses as in the example below.

Example : Set GPIB addresses as follows:

GPIB1 address : 3
GPIB2 address : 15
MC8104A address : 23
Printer address : 20

Step	Key operation	Explanation
1	System	Display the system screen.
2	[INTERFACE] F5	Display the INTERFACE function key menu.
3	[GPIB1 ADDRESS] F1	Display the current GPIB1 address.
	3 Enter	Change the GPIB1 address to 3.
4	[GPIB2 ADDRESS] F2	Display the current GPIB2 address.
	1 5 Enter	Change the GPIB2 address to 15.
5	[MC8104A ADDRESS] F3	Display the current MC8104A address.
	2 3 Enter	Set the MC8104A address to 23.
6	[RETURN] F6	Return to the MC8104A function key menu.
7	TX Test F6	Switch the screen to the transmitter tester screen.
8	Shift Copy	Display the COPY CONTROL function key menu.
	[SETUP PRINTER] F2	Display the SETUP PRINTER function key menu.
	[PRINTER ADDRESS] F5	Display the current printer address.
	2 0 Enter	Set the printer address to 20.

SECTION 3
DEVICE MESSAGE FORMAT

This section describes the format of the device messages transmitted on the bus between a controller and devices via the GPIB system.

TABLE OF CONTENTS

3.1 General Description 3-3

3.2 Program message format 3-3

3.3 Response message format 3-7

(Blank)

3.1 General Description

The device messages are data messages that are transmitted between the controller and devices. There are two types of data messages: program messages that are transferred from the controller to MS8604A (device), and response messages that are sent from MS8604A (device) to the controller. There are also two types of program commands and program queries in the program message. The program command is used to set this instrument's parameters and to instruct it to execute processing. The program query is used to query the values of parameters and measured results.

3.2 Program message format

To transfer the program messages from the controller program to MS8604A using the PRINT statement, the program message formats are defined as follows.

```
PRINT␣@1;"CF␣4GHZ"
```

Program message

When the program message is transmitted from the controller to the MS8604A, the specified terminator is attached to the end of the program message to terminate its transmission

(1) PROGRAM MESSAGE TERMINATOR

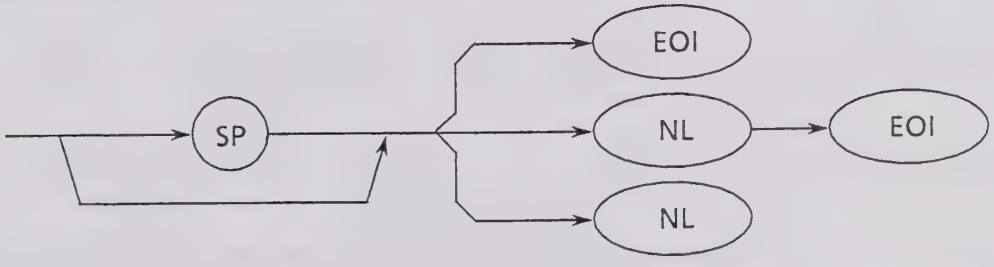

NL : Called New line or LF (Line Feed)

Carriage Return (CR) is ignored, and is not processed as a terminator.

(2) PROGRAM MESSAGE

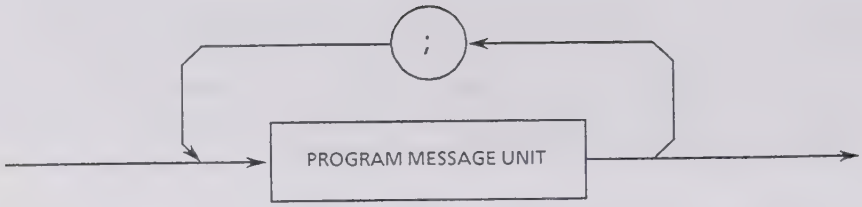

The program messages consisting of one or more program message units can be output sequentially by concatenating each of them with a semicolon.

<Example> PRINT␣@1;"CF␣1GHZ;SP␣5ØØKHZ"

(3) PROGRAM MESSAGE UNIT

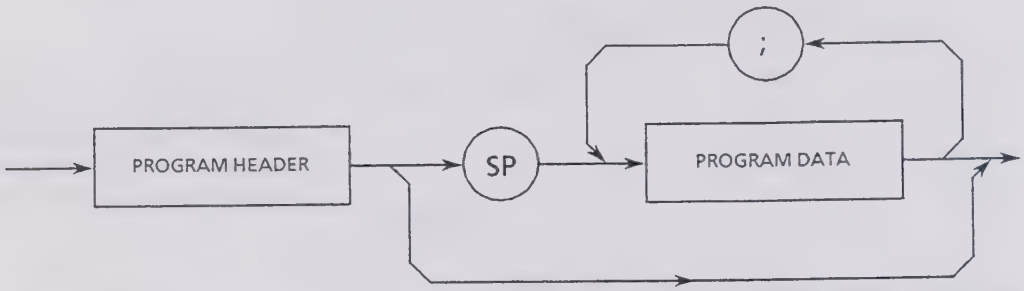

- The IEEE 488.2 common command has a leading asterisk " * " that is always placed before the program header.
- The program query has a trailing question mark " ? " that is always added at the end of the program header.

(4) PROGRAM DATA

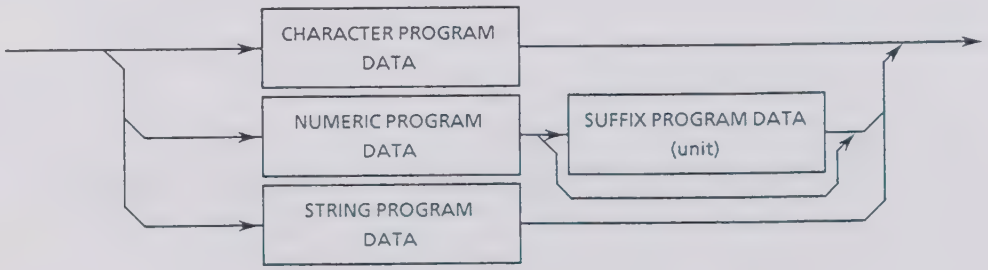

(5) CHARACTER PROGRAM DATA

Character program data consists of the upper-case alphabetic characters from A to Z, lower-case alphabetic characters from a to z, the underline of "_", and the numbers 0 to 9. They can be used in a specified combination.

<Example> PRINT␣@1;␣"ST␣AUTO" ..... Sets Sweep Time to AUTO

(6) NUMERIC PROGRAM DATA

Numeric program data has two types of formats: integer format (NR1) and fixed-point real number format (NR2).

< Integer Format (NR1) >

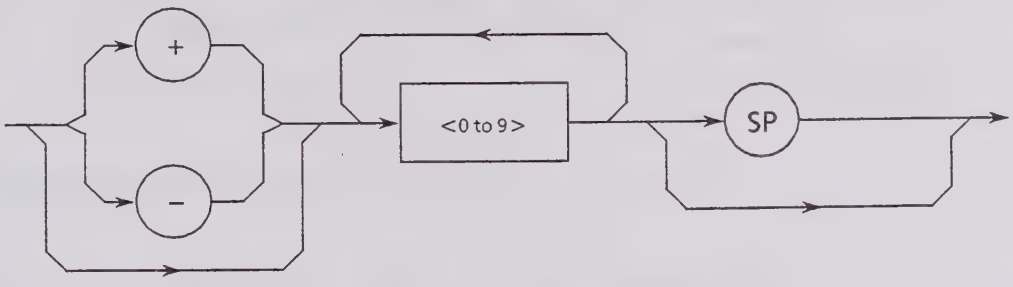

- Zeros can be inserted at the beginning → 005, +000045
- No spaces can be inserted between a + or − sign and a number → +5, + ␣5 (×)
- Spaces can be inserted after a number → +5␣␣␣
- The + sign is optional → +5, 5
- Commas cannot be used to separate digits→ 1,234,567 (×)

< Fixed-Point (real number) Format (NR2) >

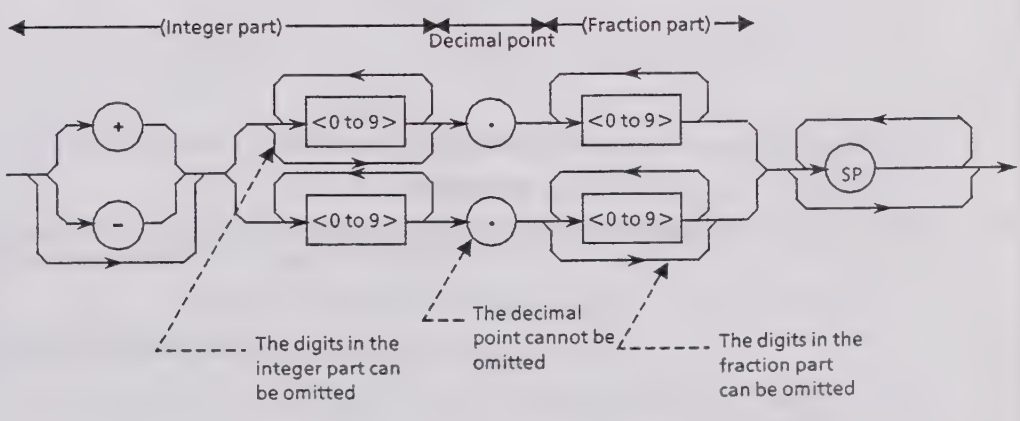

- The numeric expression of the integer format is applied to the integer part
- No spaces can be inserted between numbers and the decimal point
  → +753␣.123 (×)
- Spaces can be inserted after the digits in the fraction part → +753.123␣␣␣␣
- A number may not always be placed before the decimal point → .05
- A + or − sign can be placed before the decimal point→ +.05, −.05
- A number can end with a decimal point → 12.

(7) STRING PROGRAM DATA

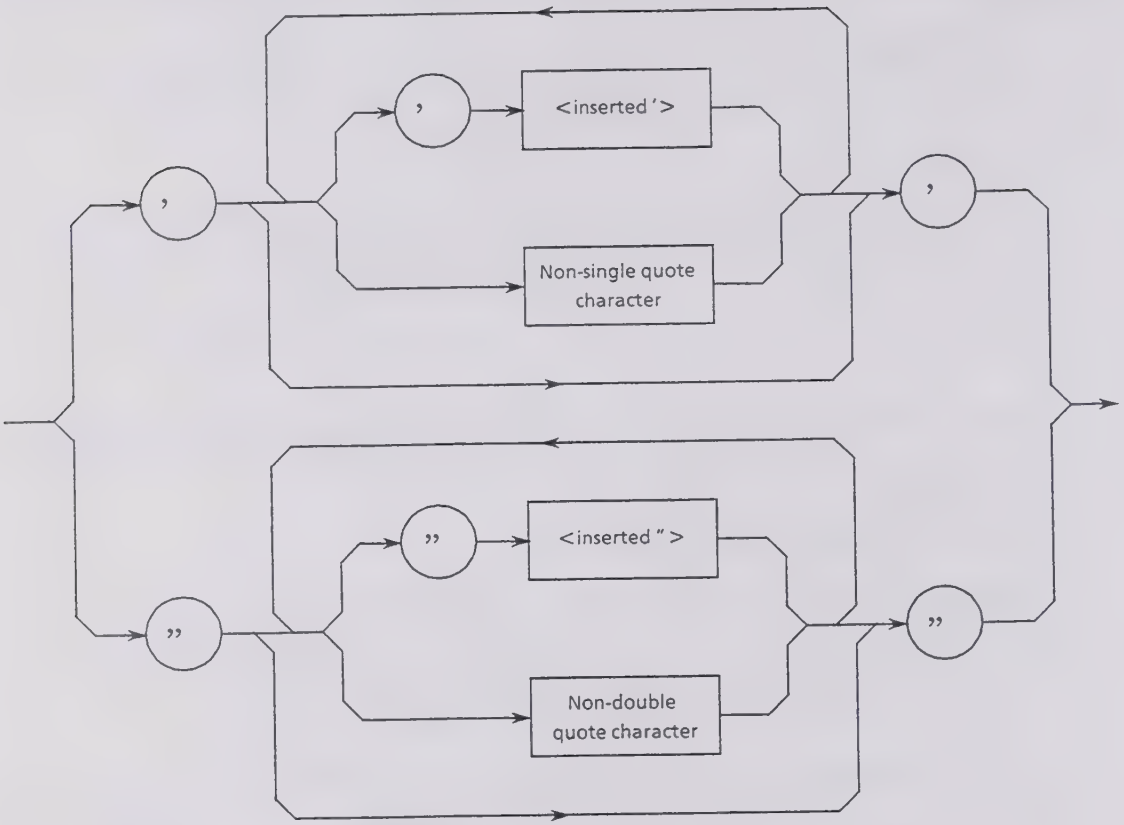

- Both ends of string program data must have a pair of single quotation marks '.....'

```
PRINT  @ 1; "TITLE 'MS86Ø4A'"
```

A single quotation mark used within the character string must be repeated as shown in "

```
PRINT  @ 1; "TITLE 'MS86Ø4A''NOISE  MEAS'''  "
```

Executing TITLE results in MS8604A 'NOISE MEAS'

Note: To use the double quotation mark " in the PRINT statement, specify CHR$ (&H22).

3.3 Response message format

To transfer the response messages from the MS8604A to the controller using the INPUT statement, the response message formats are defined as follows.

(1) RESPONSE MESSAGE TERMINATOR

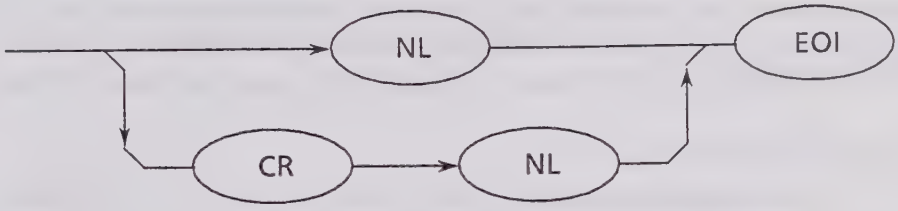

The response message terminator to be used depends on the TRM command.

(2) RESPONSE MESSAGE

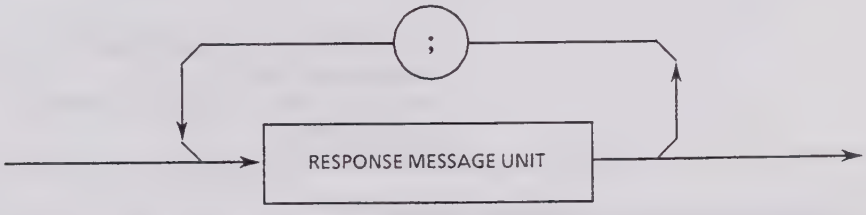

When a query is sent by the PRINT statement with one or more program queries, the response message also consists of one or more response message units.

(3) RESPONSE MESSAGE UNIT

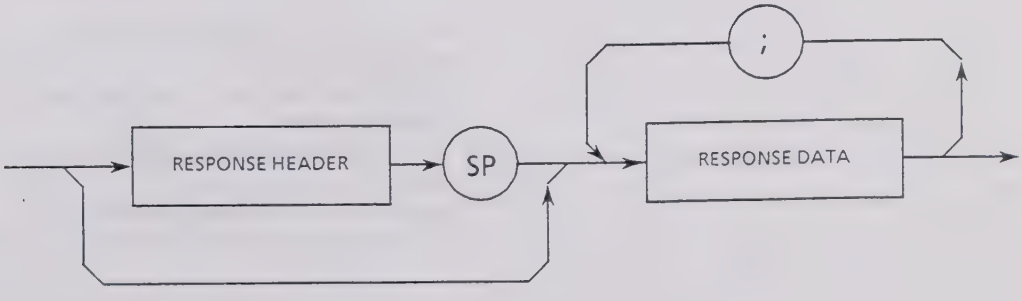

(4) RESPONSE DATA

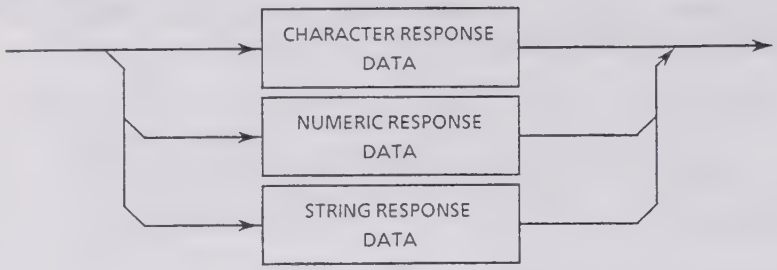

(5) CHARACTER RESPONSE DATA

Character response data consists of the upper-case alphabetic characters from A to Z, lower-case alphabetic characters from a to z, the underline "_", and the numbers 0 to 9. They can be used in a specified combination.

(6) NUMERIC RESPONSE DATA

< Integer Format (NR1) >

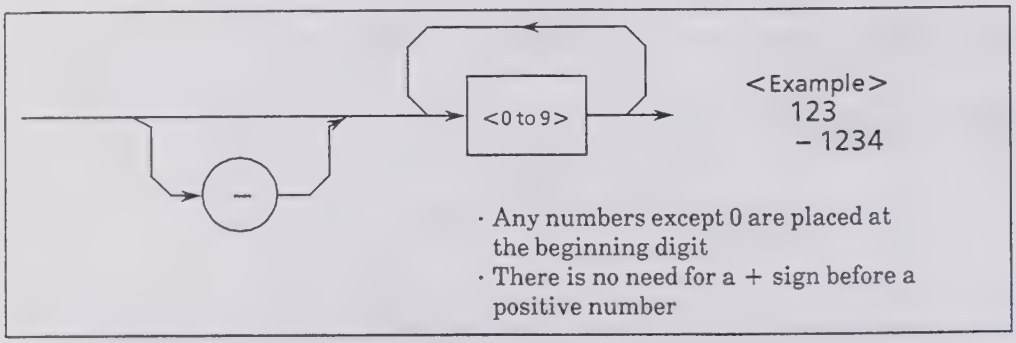

< Fixed-Point (real number) Format (NR2) >

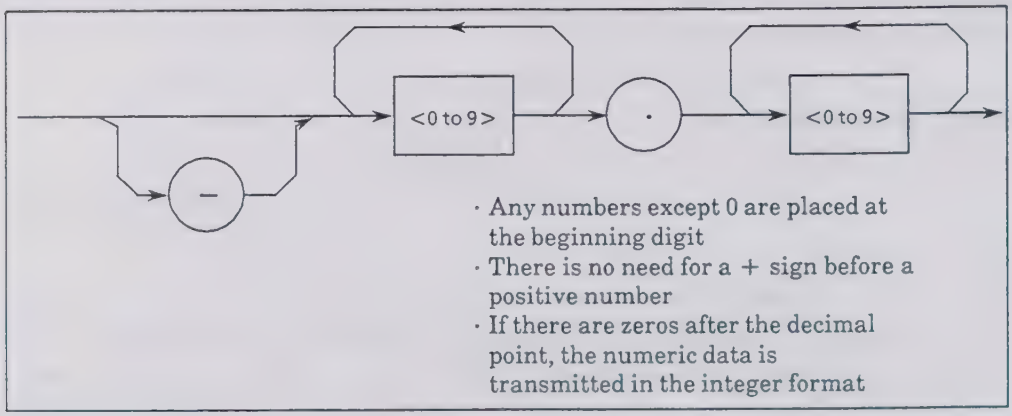

(7) STRING RESPONSE DATA

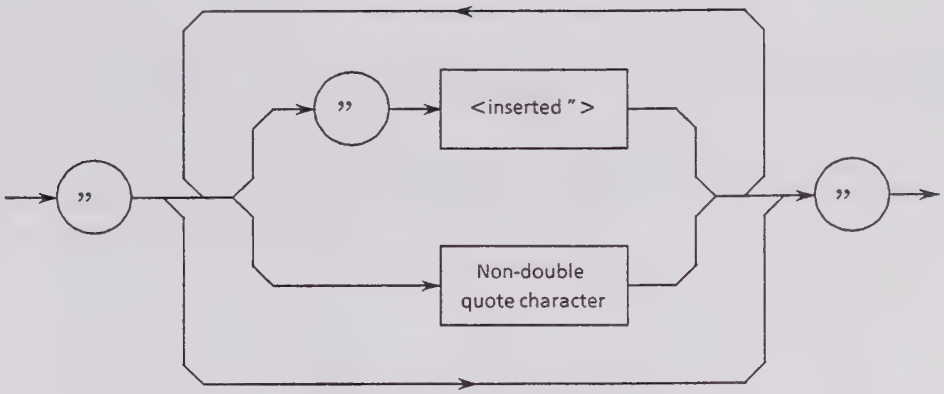

String response data is transmitted as an ASCII character string, which is enclosed with double quotation marks.

(8) Response message to input the waveform data using binary data

For binary format read and 2-bite binary data transferring, see paragraph 7.2 (4).

(Blank)

SECTION 4
STATUS MESSAGE

This section describes MS8604A status reports and their data structure and explains the techniques for synchronizing the controller and devices.

In order to obtain more detailed status information, the IEEE 488.2 standard has more common commands and common queries than the IEEE 488.1 standard. Refer to Section 6 for a detailed explanation of these common commands and queries.

TABLE OF CONTENTS

4.1 IEEE 488.2 Standard Status Model 4-4

4.2 Status Byte (STB) Register 4-6

4.2.1 ESB and MAV summary messages 4-6

4.2.2 Device-dependent summary messages 4-7

4.2.3 Reading and clearing the STB register 4-8

4.3 Enabling SRQ 4-9

4.4 Standard Event Status Register 4-10

4.4.1 Bit definition of standard event status register 4-10

4.4.2 Query error details 4-11

4.4.3 Reading, writing to and clearing the standard event status register 4-12

4.4.4 Reading, writing to and clearing the standard event status enable register 4-12

4.5 Extended Event Status Register 4-13

4.5.1 Bit definition of PTA event status register 4-14

4.5.2 Bit definition of END event status register 4-15

4.5.3 Reading, writing to and clearing the extended event status register 4-16

4.5.4 Reading, writing to and clearing the extended event status enable register 4-16

4.6 Techniques for Synchronizing MS8604A with a Controller 4-17

4.6.1 Wait for response after *OPC? query is sent 4-17

4.6.2 Wait for service request after *OPC is sent 4-18

(Blank)

The Status Byte (STB) sent by the controller is based on the IEEE 488.1 standard. The bits comprising it are called a status summary message because they represent a summary of the current data contained in registers and queues.

The following pages explain the status summary message and the structure of the status data that constitutes the status summary message bits as well as techniques for synchronizing the MS8604A and controller, which use these status messages.

4.1 IEEE 488.2 Standard Status Model

The diagram below shows the standard model for the status data structure stipulated in the IEEE 488.2 standard.

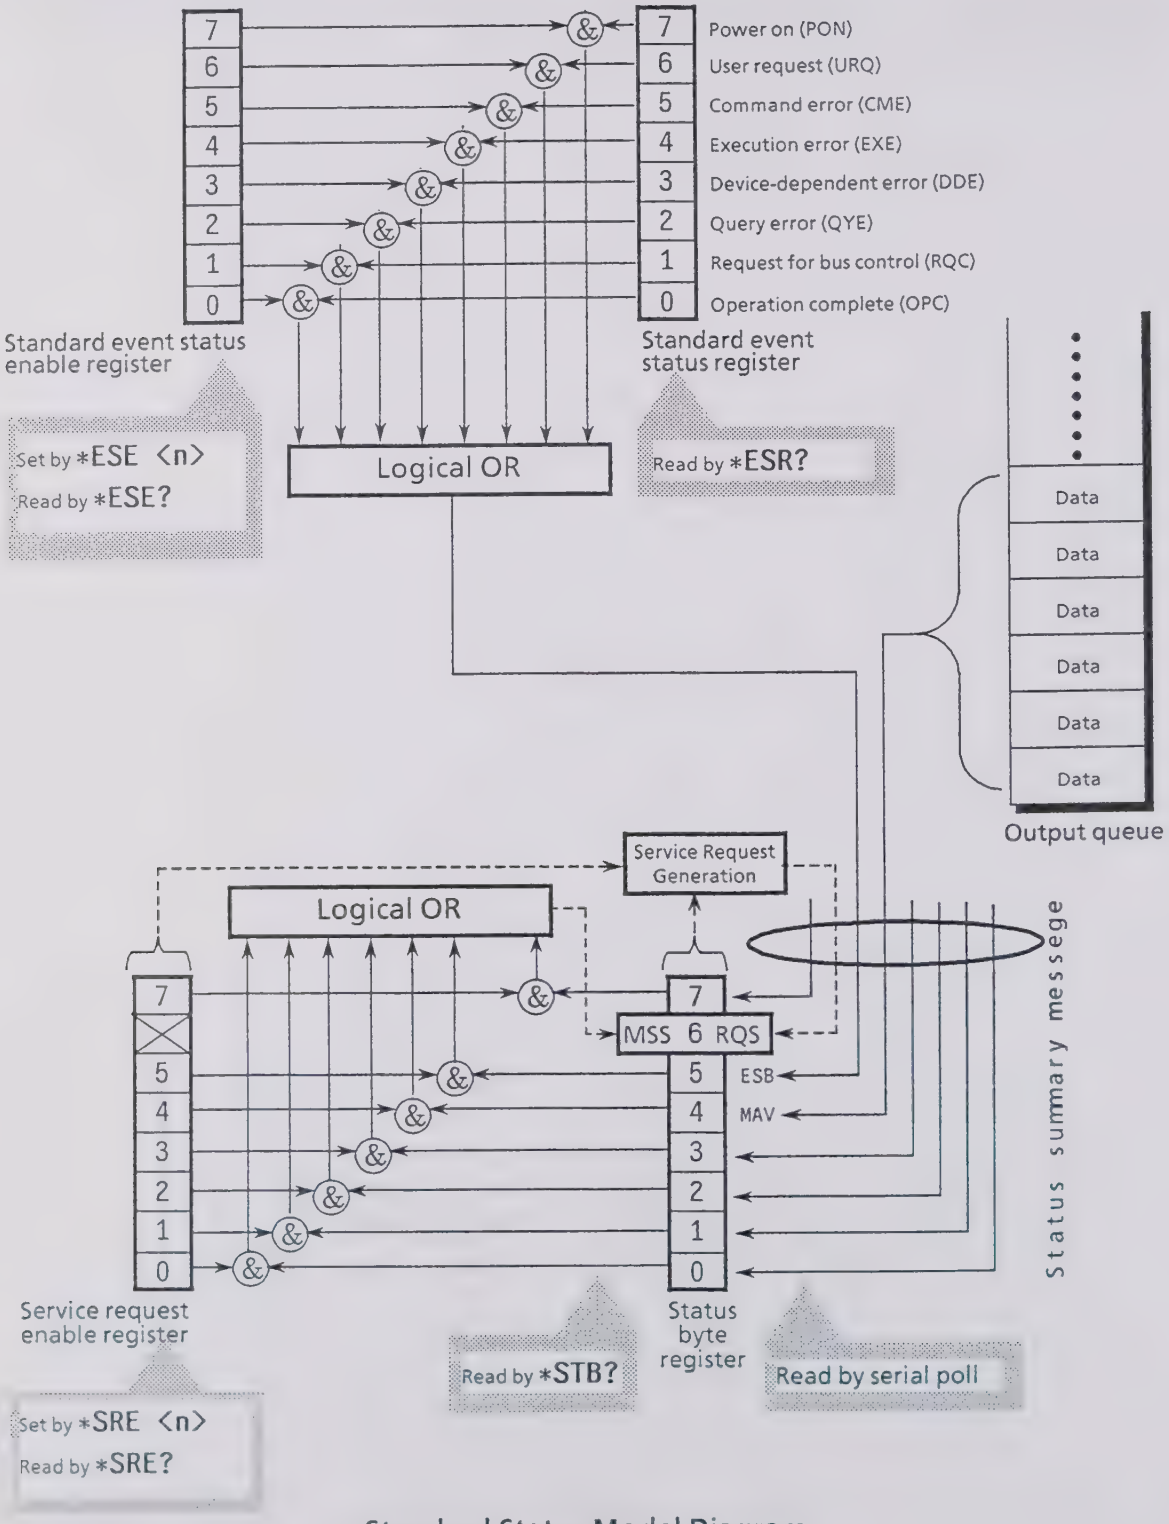

Standard Status Model Diagram

The IEEE 488.1 status byte is used in the status model. This status byte is composed of 7 summary message bits given from the status data structure. For creating the summary message bits, there are 2 models for the data structure – the register model and the queue model.

Register model	Queue model
The register model consists of the two registers used for recording events and conditions encountered by a device. These two registers are the Event Status Register and Event Status Enable Register. When the results of the AND operation of both register contents is not 0, the corresponding bit of the status bit becomes 1. In other cases, it becomes 0. And, when the result of their Logical OR is 1, the summary message bit becomes also 1. If the Logical OR result is 0, the summary message bit becomes 0 too.	The queue in the queue model is for sequentially recording the waiting status values and data. The queue structure is such that the relevant bit is set to 1 when there is data in it and 0 when it is empty.

In IEEE 488.2, there are 3 standard models for status data structure-2 register models and 1 queue model-based on the register model and queue model explained above. They are:

① Standard Event Status Register and Standard Event Status Enable Register
② Status Byte Register and Service Request Enable Register
③ Output queue

Standard Event Status Register	Status Byte Register	Output Queue
The Standard Event Status Register has the structure of the previously described register model. In this register, bits are set for 8 types of standard event encountered by a device, viz. ① Power on, ② User request, ③ Command error, ④ Execution error, ⑤ Device-dependent error, ⑥ Query error, ⑦ Request for bus control and ⑧ Operation complete. The Logical OR output bit is represented by Status Byte Register bit 5 (DIO6) as a summary message for the Event Status Bit (ESB).	The Status Byte Register is a register in which the RQS bit and the 7 summary message bits from the status data structure can be set. It is used together with the Service Request Enable Register. When the results of the OR operation of both register contents is not 0, SRQ becomes ON. To indicate this, bit 6 of the Status Byte Register (DIO7) is reserved by the system as the RQS bit which means that there is a service request for the external controller. The mechanism of SRQ conforms to the IEEE 488.1 standard.	The Output Queue has the structure of the queue model mentioned above. Status Byte Register bit 4 (DIO5) is set as a summary message for Message Available (MAV) to indicate that there is data in the output queue.

4.2 Status Byte (STB) Register

The STB register consists of device STB and RQS (or MSS) messages. The IEEE 488.1 standard defines the method of reporting STB and RQS messages but not the setting and clearing protocols or the meaning of STB. The IEEE 488.2 standard defines the device status summary message and the Master Summary Status (MSS) which is sent to bit 6 together with STB in response to an *STB? common query.

4.2.1 ESB and MAV summary messages

The following is a description of the ESB and MAV summary messages.

(1) ESB summary messages

The ESB (Event Summary Bit) summary message is a message defined by IEEE 488.2, which is represented by bit 5 of the STB register. This bit indicates whether at least one of the events defined in IEEE 488.2 has occurred or not when the service request enable register is set so that events are enabled after the final reading or clearing of the standard event status register. The ESB summary message bit becomes true when the setting permits events to occur if any one of the events recorded in standard event status register is true. Conversely, it is false if none of the recorded events occurs even if events are set to occur.
When the ESR register was read by the *ESR? query and when the ESR register was cleared, this bit becomes FALSE (0).

(2) MAV summary messages

The MAV summary message is a message defined in IEEE 488.2 and represented by bit 4 in the STB register. This bit indicates whether the output queue is empty or not. The MAV summary message bit is set to 1 (true) when a device is ready to receive a request for a response message from the controller and to 0 (false) when the output queue is empty. This message is used to synchronize the exchange of information with the controller. For example, it can be used get the controller to wait till MAV is true after it has sent a query command to a device. While the controller is waiting for a response from the device, it can process other jobs. Reading the output queue without first checking MAV will cause all system bus operations to be delayed until the device responds.

4.2.2 Device-dependent summary messages

The IEEE 488.2 standard does not specify whether bits 7 (DIO8) and 3 (DIO4) to 0 (DIO1) of the status byte register are used as status register summary bits, or used to indicate that there is data in a queue. These bits can be used as device-dependent summary messages.

Device-dependent summary messages have the respective status data structures of the register model or the queue model. Thus, the status data structure may be either the register to report events and status in parallel or the queue to report conditions and status in sequence. The summary bit represents a summary of the current status of the corresponding data structure. In the case of the register model, the summary bit is true when there is an event set to permit the occurrence of more than one true; while in the case of the queue model, it is true if the queue is not empty.

As shown below, the MS8604A does not use bits 0, 3 and 7. As it uses bits 1 and 2 as the summary bits of the status register, it has 3 register model types (, where 2 types extended) and one queue model type-an output queue with no extension.

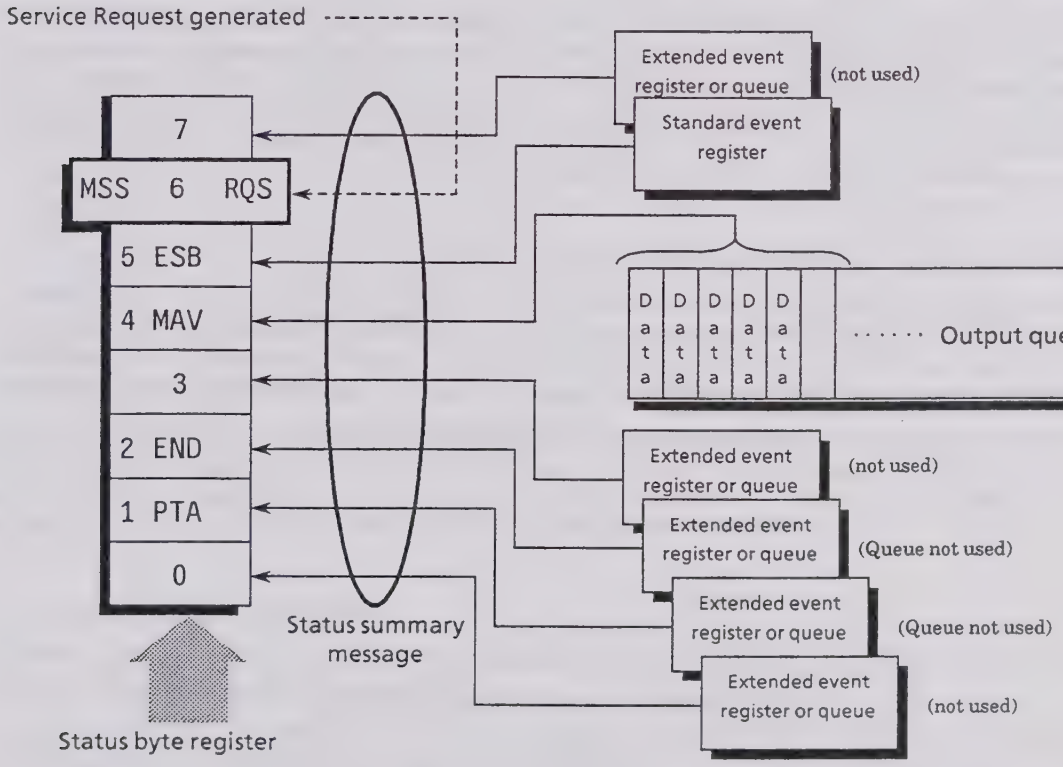

4.2.3 Reading and clearing the STB register

Serial poll or the *STB? common query are used to read the contents of STB register. STB messages conforming to IEEE 488.1 can be read by either method, but the value sent to bit 6 is different for each of them.
The STB register can be cleared using the *CLS command.

(1) Reading by serial poll

When using the serial poll conforming to IEEE 488.1, the device must return a 7-bit status byte and an RQS message bit which conforms to IEEE 488.1. According to IEEE 488.1, the **RQS** message indicates whether the device sent **SRQ** as true or not. The value of the status byte is not changed by serial poll. The device must set the RQS message to false immediately after being polled. As a result, if the device is again polled before there is a new cause for a service request, the **RQS** message is false.

(2) Reading by the *STB common query

The *STB? common query requires the device to send the contents of the STB register and one integer format response message from the MSS (Master Summary Status) summary message. The response represents the total binary weighted value of the STB register and the **MSS** summary message. The STB-register bits 0 to 5 and 7 are weighted to 1, 2, 4, 8, 16, 32, and 128; and the **MSS** to 64, respectively. Thus, excepting the fact that bit 6 represents the MSS summary message instead of the **RQS** message, the response to *STB? is identical to that for serial poll.

(3) Definition of MSS (Master Summary Status)

MSS indicates that there is at least one cause for a service request. The MSS message is represented at bit 6 in a device response to the *STB? query but it is not produced as a response to serial poll. In addition, it is not part of the status byte specified by IEEE 488.1. **MSS** is produced by the logical OR operation of STB register with SRQ enable (SRE) register. In concrete terms, MSS is defined as follows.

(STB Register bit 0 AND SRE Register bit 0)
OR
(STB Register bit 1 AND SRE Register bit 1)
OR
:
:
(STB Register bit 5 AND SRE Register bit 5)
OR
(STB Register bit 7 AND SRE Register bit 7)

As bit-6 status of the STB and SRQ enable registers are ignored in the definition of MSS, it can be considered that bit-6 status are always being 0 when calculating the value of MSS.

(4) Clearing the STB register by the *CLS common command

With the exception of the output queue and its **MAV** summary message, the *CLS common command clears all status data structures (status event registers and queues) as well as the summary messages corresponding to them.

The *CLS command does not affect settings in the enable registers.

4.3 Enabling SRQ

All types of summary message in the STB register can be enabled or disabled for service requests by using the SRQ enable function. The service request enable (SRE) register is used for this function to select summary messages as shown in the diagram below.

Bits in the service request enable register correspond to bits in the status byte register. If a bit in the status byte corresponding to an enabled bit in the service request enable register is set to 1, a device makes a service request to the controller with the RQS bit set to 1. For example, if bit 4 (MAV) in the service request enable register is enabled, the device makes a request for service to the controller each time the MAV bit is set to 1 when there is data in the output queue.

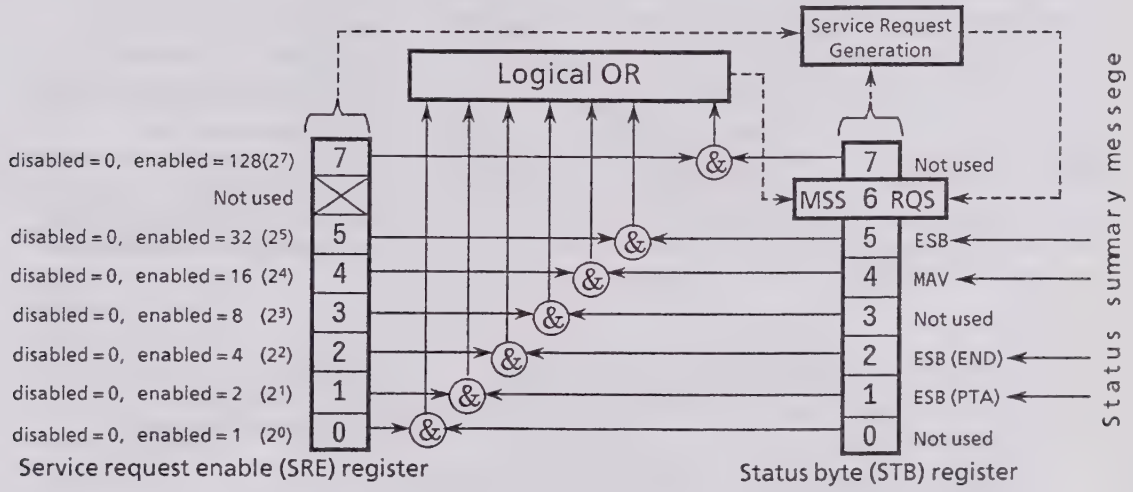

(1) Reading the SRE register

The contents of the SRE register are read using the ***SRE?** common query. The response message to this query is an integer from 0 to 255 which is the sum of the bit digit weighted values in the SRE register. SRE register bits 0 to 5 and 7 are respectively weighted to 1, 2, 4, 8, 16, 32 and 128. The unused bit 6 must always be set to 0.

(2) Updating the SRE register

The ***SRE** common instruction is used to write data in the SRE register. An integer from 0 to 255 is added after the ***SRE** common instruction.

This integer indicates the total number of bits in the SRE register (weighted values: 1, 2, 4, 8, 16, 32, and 128), and sets the corresponding SRE register bits to 0 or 1.

A bit value of 1 indicates an enabled state and 0 indicates a disabled state. Ignore the value of bit 6.

4.4 Standard Event Status Register

4.4.1 Bit definition of standard event status register

The standard event status register must be available on all devices conforming to the IEEE 488.2 standard. The diagram below shows the operation of the standard event status register model. Because the operation of the model is the same as that for the other models explained up till now, the following only explains the meaning of each bit in the standard event status register as defined in the IEEE 488.2 standard.

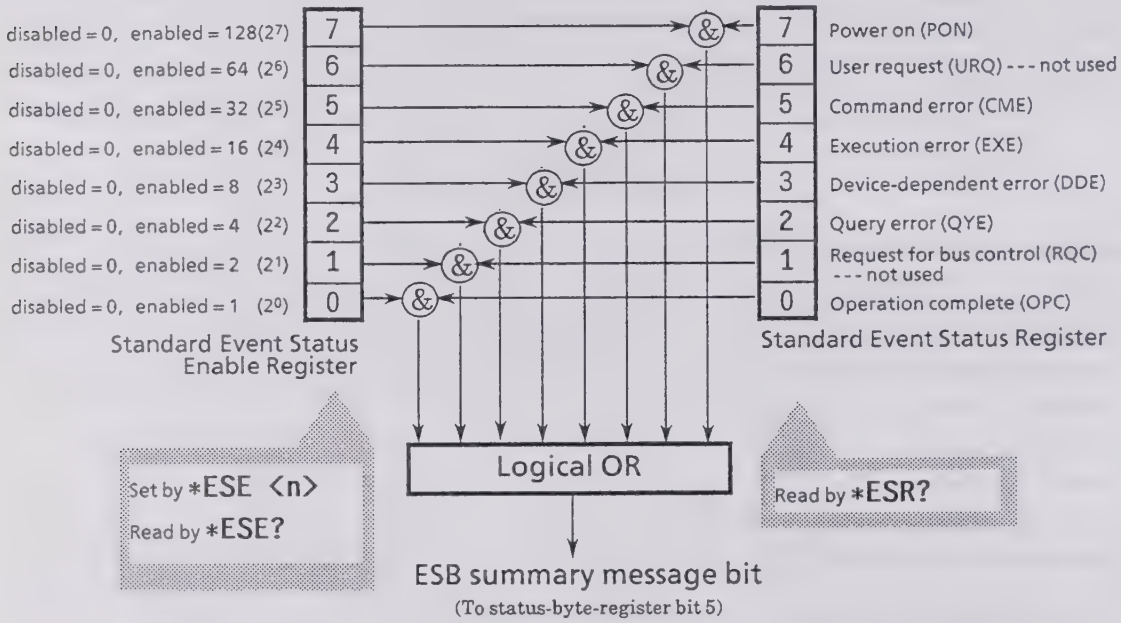

The left side standard event status enable (ESE) register selects whether the register makes the summary message true or not when the corresponding event status register becomes 1.

Bit	Event name	Description
7	PON : Power on	The power is turned to on.
6	URQ : User Request	Request for local control (rtl). This bit is produced regardless of whether a device is in remote or local mode. It is not used for the MS8604A so, it is always set to 0.
5	CME : Command Error	An illegal program message, a misspelt command or a GET command within a program is received.
4	EXE : Execution Error	A legal program message, which cannot be executed, is received.
3	DDE : Device-dependent Error	An error caused by other than CME, EXE or QYE occurred.
2	QYE : Query Error	An attempt is made to read data in the output queue though there is none there, or data is lost from the output queue due to any reason, e.g. overflow etc..
1	RQC : Request Control	A device is requesting control of the bus. This bit is not used on the MS8604A so, it is always set to 0.
0	OPC : Operation Complete	A device has completed operations which were pending and is ready to receive new commands. This bit is only set in response to the *OPC command.

4.4.2 Query error details

No.	Item	Description
1	Incomplete program messages	If a device receives an MTA from the controller before it receives the terminator of the program message it is receiving, it aborts the incomplete program message and waits for the next one. In order to abort the incomplete message, the device clears its input buffer and output queue, reports a query error and sets bit 2 in the standard status register to indicate the query error.
2	Interruption of response message	If a device receives an MLA from the controller before it has sent the terminator of the response message it is sending, it automatically interrupts the response message and waits for the next program message. In order to interrupt the response message, the device clears its output queue, reports a query error and sets bit 2 in the standard status register to indicate the query error.
3	Sending the next program message without reading the previous response message	When a device becomes unable to send a response message because the controller has sent another program message immediately following a program or query message, the device aborts the response message and waits for the next program message. It then reports a query error as in No. 2 above.
4	Output queue overflow	When several program and query messages are executed in succession, there may be too many response messages for the output queue (256 bytes). If further query messages are received when the output queue is full, the output queue cannot send responses to them because an overflow situation exists in it. If there is an overflow in the output queue, the device clears it and resets the section where response messages are created. Then it sets bit 2 in the standard event status register to indicate a query error.

4.4.3 Reading, writing to and clearing the standard event status register

Reading	The register is destructively read by the *ESR? common query, i.e. it is cleared after being read. The response message is an integer format data (NR1) value obtained by binary weighting the event bit and converting it to a decimal number.
Writing	With the exception of clearing, writing operations cannot be performed externally.
Clearing	The register is only cleared in the following cases. ① A *CLS command is received ② The power is turned on when the power-on-status-clear flag is true. Devices (for which the power-on sequence is being executed) first clear their standard event status registers but later record events that occurred during the sequence in them. (e.g. the setting of the PON event bit, etc.) ③ An event is read for the *ESR? query command

4.4.4 Reading, writing to and clearing the standard event status enable register

Reading	The register is non-destructively read by the *ESE? common query, i.e. it is not cleared after being read. The response message is returned by an integer format data (NR1) after having been binary weighted and converted to decimal.
Writing	The register is written to by the *ESE common command. As bits 0 to 7 of the register are respectively binary weighted to 1, 2, 4, 8, 16, 32, 64 and 128; data to be written is sent by <DECIMAL NUMERIC PROGRAM DATA> which is the digit total of the bits selected from these bits.
Clearing	The register is cleared in the following cases. ① A *ESE command with a data value of 0 is received ② When the power is turned on when the power-on-status-clear flag is true. The event status enable register is not affected by the following. ① Changes of the status of the IEEE 488.1 device clear function ② A *RST common command is received ③ A *CLS common command is received

4.5 Extended Event Status Register

The register models of the status byte register, standard event status register and enable registers are mandatory for equipment conforming to the IEEE 488.2 standard.

In IEEE 488.2, status-byte-register bits 7 (DIO8), 3 (DIO4) to 0 (DIO1) are assigned to status-summary bits supplied by the extended-register and extended-queue models.

For the MS8604A, as shown in the diagram below, bits 7, 3 and 0 are unused and bits 1 and 2 are assigned to the END and PTA summary bits as the status-summary bits supplied by the extended-register model. As the queue model is not extended, there is only one type of queue-the output queue.

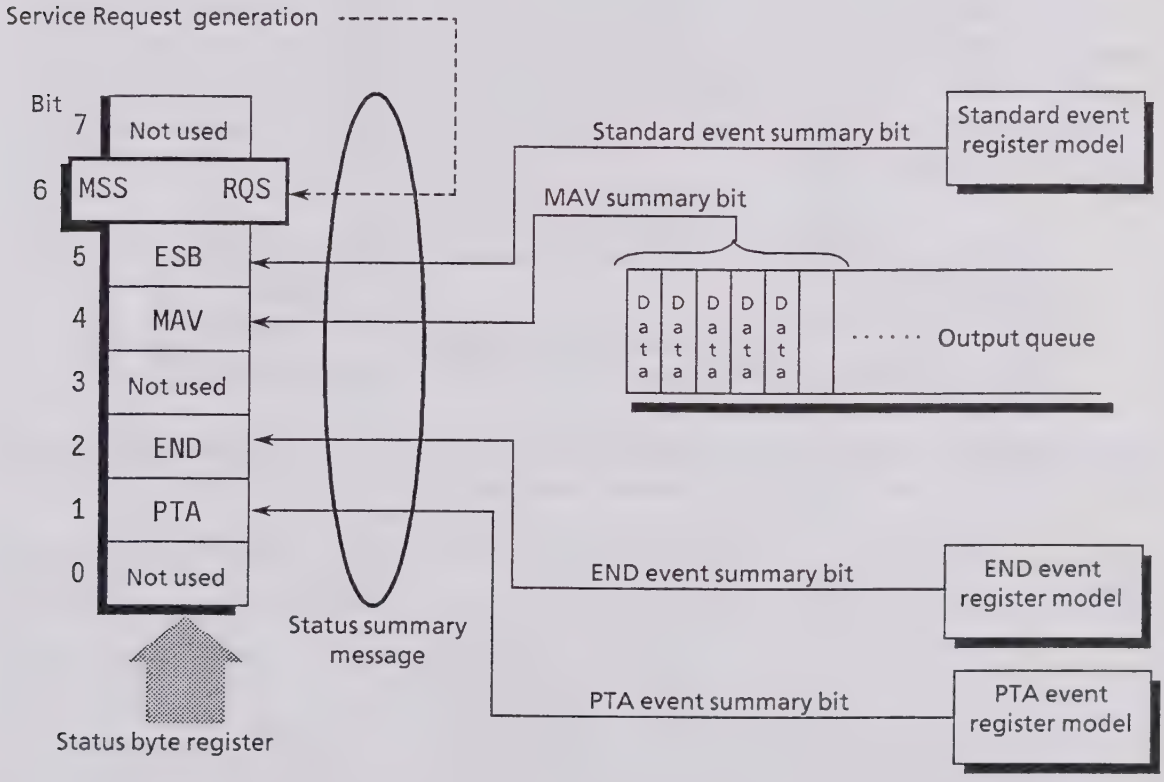

The following pages describe bit definition, the reading, writing to and clearing of registers for the PTA and END extended event register models.

4.5.1 Bit definition of PTA event status register

The following describes the operation of the PTA event status register model, the naming of its event bits and what they mean.

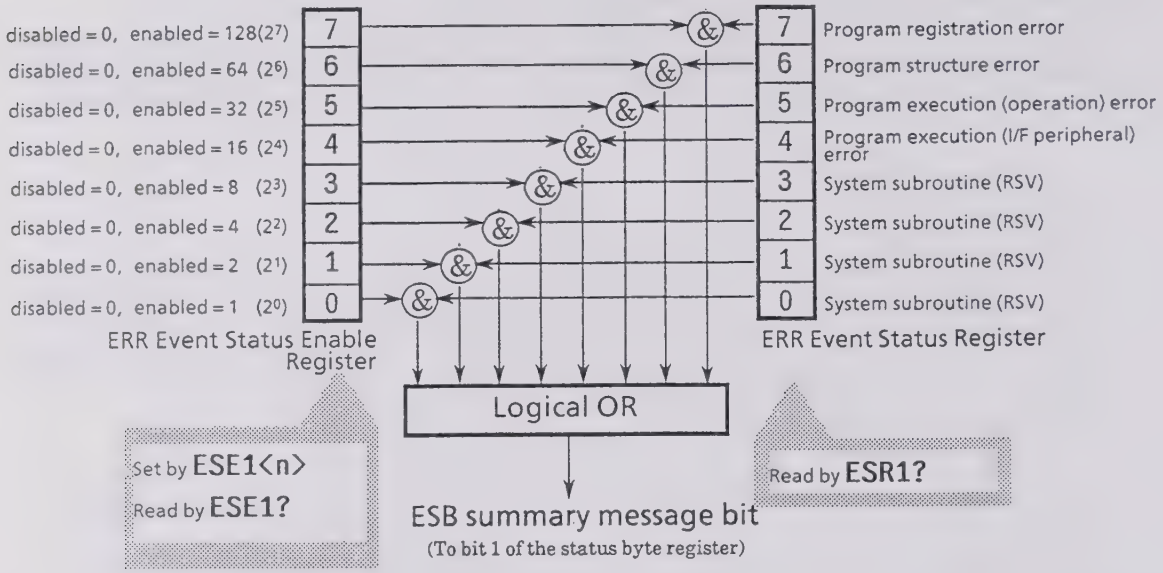

The left side PTA ivent status enable register selects whether the register makes the summary message true or not when the corresponding event status register becomes 1.

Bit	Event name	Description
7	Registration error	Error at program registration
6	Structure error	Error on program structure
5	Execution (operation) error	Error at operation on program execution
4	Execution (I/F etc.) error	Error at other than program operation
3	SRQ send	┐
2	SRQ send	Used for sending service request with PTA subroutine
1	SRQ send	CALL RSV (n)
0	SRQ send	┘

4.5.2 Bit definition of END event status register

The following describes the operation of the END event status register model, the naming of its event bits and what they mean.

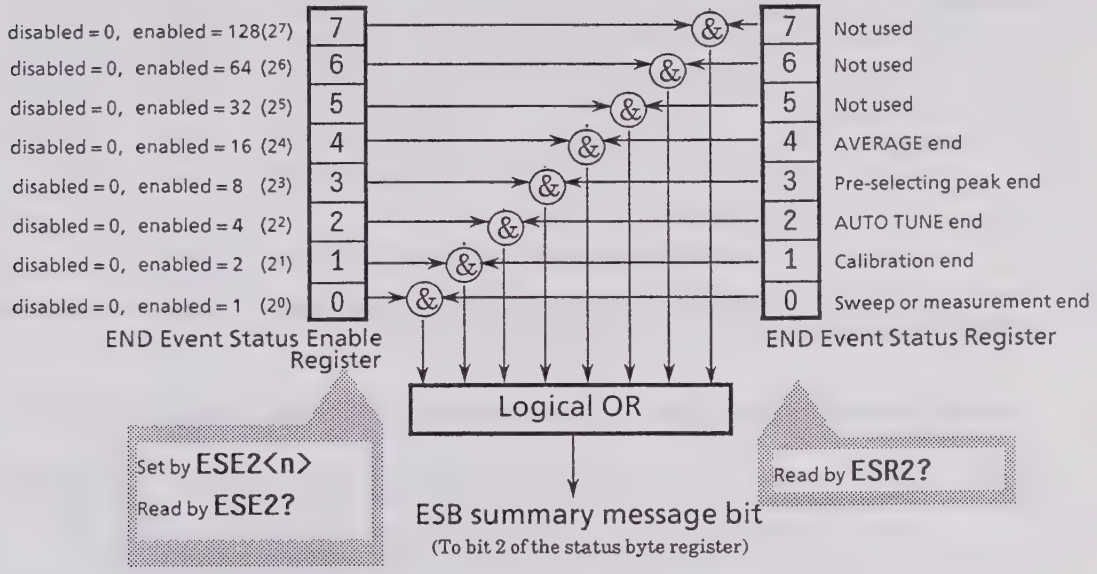

The left side END ivent status enable register selects whether the register makes the summary message true or not when the corresponding event status register becomes 1.

Bit	Event name	Description
7	(Not used)	(Not used)
6	(Not used)	(Not used)
5	(Not used)	(Not used)
4	AVERAGE end	This bit is set to 1 when averaging terminates.
3	Pre-selecting peak end	This bit is set to 1 when pre-selecting peak terminates.
2	AUTO TUNE end	This bit is set to 1 when AUTO TUNE processing terminates.
1	CAL end	This bit is set to 1 when calibration terminates.
0	Sweep or measurement end	This bit is set to 1 when sweep or measurement terminates.

4.5.3 Reading, writing to and clearing the extended event status register

Reading	The register is destructively read by the a query, i.e. it is cleared after being read. The PTA and END event status registers are read by the ESR1? and ESR2? queries. The read value, an integer format data (NR1), is obtained by binary weighting the event bit and converting it to decimal.
Writing	With the exception of clearing, writing operations cannot be performed externally.
Clearing	The register is cleared in the following cases. ① A *CLS command is received ② The power is turned on when the power-on-status-clear flag is true. ③ An event is read for a query command

4.5.4 Reading, writing to and clearing the extended event status enable register

Reading	The register is non-destructively read by a query, i.e. it is not cleared after being read. The PTA and END event status registers are read by the ESE1? and ESE2? queries. The read value, returned by an integer format data (NR1), is obtained by binary weighting the event bit and converting it to decimal.
Writing	The PTA and END event status registers are written to by the ESE1 and ESE2 program commands. As bits 0 to 7 of the registers are respectively binary weighted to 1, 2, 4, 8, 16, 32, 64 and 128, data to be written is sent by <DECIMAL NUMERIC PROGRAM DATA>, the digit total weighted value of the bits selected from among them.
Clearing	The register is cleared in the following cases. ① ESE1 and ESE2 program commands with a data values of 0 are received by the PTA and END event status registers. ② When the power is turned on when the power-on-status-clear flag is true. The extended event status enable register is not affected by the followings: ① Changes of the status of the IEEE 488.1 device clear function ② A *RST common command is received ③ A *CLS common command is received

4.6 Techniques for Synchronizing MS8604A with a Controller

The MS8604A usually treats program messages as sequential commands that do not execute the processing of newly-received commands until the previous command has been processed. Thus, special consideration need not be taken for pair-synchronization between MS8604A and the controller.

If the controller controls one or more devices and synchronizes with them, after all the commands specified for the MS8604A have been processed, the next commands must be sent to other devices.

There are two ways of synchronizing the MS8604A with the controller.

① Wait for a response after ***OPC?** query is sent

② Wait for SRQ after ***OPC** is sent

4.6.1 Wait for response after *OPC? query is sent

The MS8604A outputs " 1 " as the response message when executing the ***OPC?** query command. The controller is synchronized with the MS8604A by waiting for the response message to be entered.

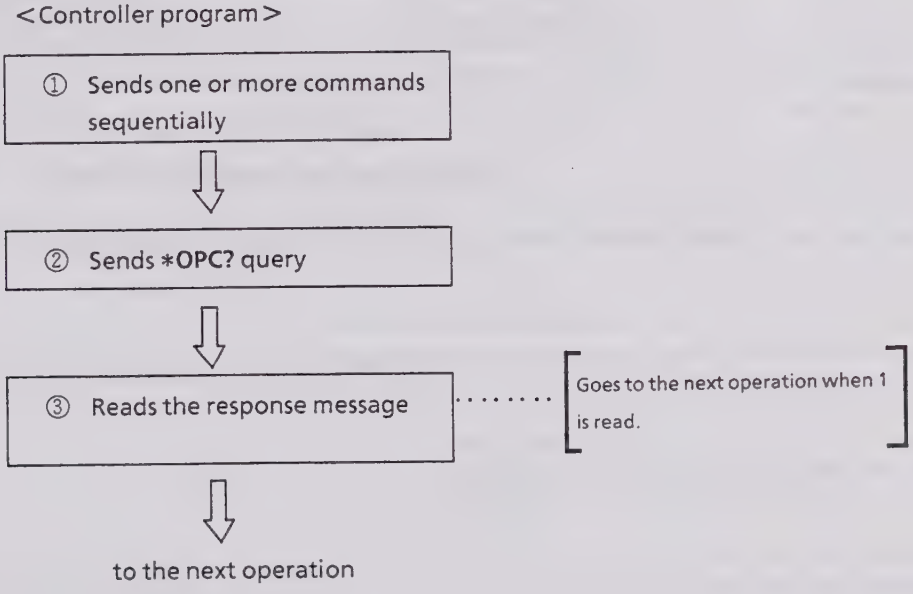

4.6.2 Wait for service request after *OPC is sent

The MS8604A sets the operation-complete bit (bit 0) to 1 when executing the ***OPC** command. The controller is synchronized with the MS8604A by waiting for SRQ when the operation-complete bit is set for SRQ.

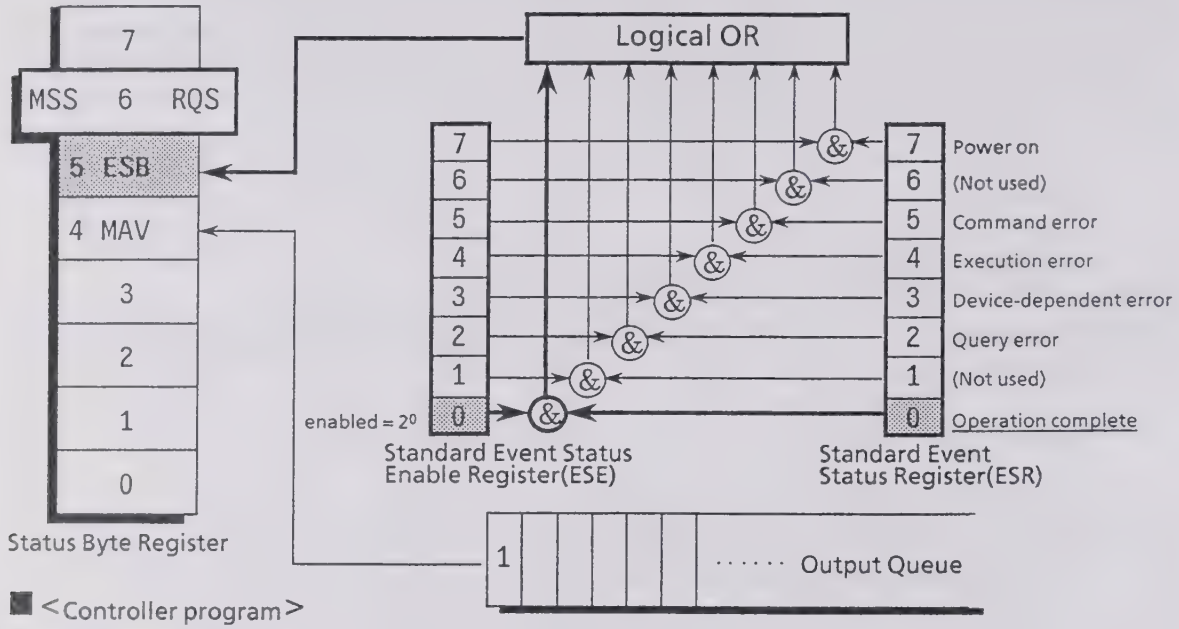

■ <Controller program>

① Enables the 2^0 bit (1) of the Standard Event Status Enable Register — `PRINT␣@1;"*ESE␣1"`

⇩

② Enables the 2^5 bit (32) of the Service Request Enable Register — `PRINT␣@1;"*SRE␣32"`

⇩

③ Makes the device execute the specified operation

⇩

④ Sends the *OPC command — `PRINT␣@1;"*OPC"`

⇩

⑤ Wait for an SRQ interrupt (ESB summary message) — · · · · Value of status byte: $2^6 + 2^5 = 96$

SECTION 5
INITIAL SETTINGS

There are 3 levels of initialization for the GPIB interface system.
The first level is bus initialization in which the system bus is in the idle state.
The second level is initialization for message exchange in which devices are able to receive program message.
The third level is device initialization in which device functions are initialized.
These levels of initialization prepare a device for operation.

TABLE OF CONTENTS

5.1 Bus Initialization by the IFC Statement 5-4

5.2 Initialization for Message Exchange by DCL and SDC Bus Commands 5-5

5.3 Device Initialization by the *RST Command 5-6

5.4 Device Initialization by the PRE/INI/IP Command 5-7

5.5 Device Status at Power-on 5-8

(Blank)

In the IEEE 488.2 standard, the initialization levels are stipulated to be divided into three: the first level is " bus initialization ", the second level is " initialization for message exchange ", and the third level is " device initialization ". This standard also stipulates that a device must be set to a known state when the power is turned on.

Level	Initialization type	Description	Level combination and sequence
1	Bus initialization	The **IFC** message from the controller initializes all interface functions connected to the bus.	Can be combined with other levels, level 1 must be executed before level 2.
2	Initialization for message exchange	The message exchanges of all devices and specified devices on the GPIB are initialized respectively by the **DCL** (Device Clear) and **SDC** (Selected Device Clear) GPIB bus commands, which also nullify the function that reports to the controller that operation has completed.	Can be combined with other levels, level 2 must be executed before level 3.
3	Device initialization	The ***RST** or **PRE/INI/IP** command returns the specified device to the device-dependent known state, regardless of the conditions under which they were previously being used.	Can be combined with other levels, level 3 must be executed after levels 1 and 2.

The following paragraph describes the commands for executing levels 1, 2, and 3 and the items that are initialized by the execution. It also describes the known state which is set when the power is switched on.

5.1 Bus Initialization by the IFC Statement

■ Example

```
ISET␣IFC
```

■ Explanation

The **IFC** statement initializes the interface functions of all devices connected to the GPIB bus line.

The initialization of interface functions involves erasing the settings made by the controller and resetting them to their initial states. In the table below, ○ indicates the functions which are initialized; △ indicates the functions which are partially initialized.

No	Function	Symbol	Initialization by IFC
1	Source handshake	SH	○
2	Acceptor handshake	AH	○
3	Talker or extended talker	T or TE	○
4	Listener or extended listener	L or LT	○
5	Service request	SR	△
6	Remote/local	RL	
7	Parallel poll	PP	
8	Device clear	DC	
9	Device trigger	DT	
10	Controller	C	○

Bus initialization by the **IFC** statement does not affect the device-operating state (frequency settings, lamp on/off, etc).

5.2 Initialization for Message Exchange by DCL and SDC Bus Commands

■ Example

`WBYTE␣&H3F,␣&H14;`	Initializes all devices under the bus for message exchange (sending DCL)
`WBYTE␣&H3F,`	Initializes only the device whose address is 3 for message exchange (sending SDC)

■ Explanation

This statement executes the initialization for message exchange of all devices or only the specified device on the GPIB of the specified select code.

■ Items to be initialized for message exchange

The MS8604A by which the DCL or SDC bus command is accepted executes the following.

① Input buffer and Output Queue	Cleared, at the same time the MAV bit is also cleared.
② Parser, Execution Controller, and Response Formatter	Reset
③ Device commands including *RST	Clears all commands that prevent these commands from executing.
④ Processing the *OPC command	Puts a device in OCIS (Operation Complete Command Idle State). As a result, the operation complete bit cannot be set in the Standard Event Status Register.
⑤ Processing the *OPC? query	Puts a device in OQIS (Operation Complete Query Idle State). As a result, the operation complete bit 1 cannot be set in the Output Queue.

Note: The items listed below are not affected even if processing the DCL and SDC commands is executed.

① The current data set or stored in the device.

② Front panel settings.

③ Other status byte state except MAV bit.

④ Device operation in progress.

5.3 Device Initialization by the *RST Command

■ Syntax

```
*RST
```

■ Example

```
PRINT␣@1;"*RST" ..... Initializes the device (MS8604A) whose address is 1 with level 3
```

■ Explanation

The *RST (Reset) command is an IEEE 488.2 common command which resets a device with level 3.

The *RST (Reset) command is used to reset a device (MS8604A) to a specific initial state. Refer to the separate volume " Panel Operation Appendix B " for details of initialization items and initial values.

Note: The *RST command does not affect the items listed below.

① IEEE 488.1 interface state
② Device address
③ Output Queue
④ Service Request Enable register
⑤ Standard Event Status Enable register
⑥ Power-on-status-clear flag setting
⑦ Calibration data affecting device specifications
⑧ Parameters preset for controlling external devices etc

5.4 Device Initialization by the PRE/INI/IP Command

■ Syntax

```
PRE
INI
IP
```

■ Example (program message)

```
PRINT␣@1;"PRE" ..... Initializes the device (MS8604A) whose address is 1 with level 3
```

■ Explanation

The PRE/INI, and IP commands are MS8604A device-dependent messages which initialize a device with level 3.

Refer to the separate volume " Panel Operation Appendix B " for details of items initialized by the PRE, INI, and IP commands and initial values.

5.5 Device Status at Power-on

When the power is switched on:

① The device is set to the status before the last power off.

② The Input Buffer and Output Queue are cleared.

③ The Parser, Execution Controller, and Response Formatter are initialized.

④ The device is put into the OCIS (Operation Complete Command Idle State).

⑤ The device is put into the OQIS (Operation Complete Query Idle State).

⑥ The Standard Event Status and Standard Event Status Enable Registers are cleared. Events can be recorded after the registers have been cleared.

For the special case of ①, when the power supply is first turned on after the device is shipped, the initial values are set to those in the initial setting table (refer to the separate volume " Panel Operation Appendix B).

SECTION 6
DETAILS OF DEVICE MESSAGES

This section lists the device messages in alphabetic order and describes their functions. The device messages are classified into four types; IEEE 488.2 common commands, MS8604A common commands, TX Test mode commands, and spectrum mode commands.

TABLE OF CONTENTS

6.1 IEEE 488.2 common commands 6-7
*CLS 6-8
*ESE 6-8
*ESR? 6-9
*IDN? 6-9
*OPC 6-10
*OPC? 6-10
*PCB 6-11
*PSC 6-11
*PSC? 6-12
*RST 6-12
*SRE 6-13
*STB? 6-13
*TRG 6-14
*TST? 6-14
*WAI 6-15

6.2 MS8604A common commands 6-16
ALARM 6-17
BAUD 6-17
BEP 6-18
BIN 6-18
BZR 6-19
CONTS 6-19
DATE 6-20
DSPL 6-20
DTAB 6-21
ESE1 6-21
ESE2 6-22
ESR1? 6-22
ESR2? 6-23
GPIA 6-23
GTOUT 6-24
INI 6-24
IP 6-25
KSE 6-25
MC8104 6-26
PLS 6-26
PMCS 6-27
PMOD 6-27
PNLMD 6-28
PRE 6-28
PRIA 6-29
PRINT 6-29
PRTY 6-30
RC 6-30
RCM 6-31
RDATA 6-31
RFINPUT 6-32
RGDIR 6-32
RGRC 6-33
RGSV 6-33
SNGLS 6-34
STPB 6-34
SV 6-35
SVM 6-35
SWP 6-36
S1 6-36
S2 6-37
TIME 6-37
TITLE 6-38
TOUT 6-38
TRM 6-39
TTL 6-39

TABLE OF CONTENTS (Continued)

XMA 6-40
XMB 6-40
XMC 6-41
XMD 6-41
XME 6-42
XMT 6-42

6.3 TX Test commands 6-44
ADJCH? 6-45
ADJMEAS 6-46
AUNITS 6-46
AUTORNG 6-47
AVR 6-47
BITR? 6-48
BITRERR? 6-48
BPATT 6-49
BS 6-49
BSTAVG 6-50
CALADJ 6-50
CALOSC 6-51
CARRF? 6-51
CARRFERR? 6-52
CDJ 6-52
CF 6-53
CHAN 6-53
CHCARR 6-54
CHFREQ 6-54
CHNUM 6-55
CHSPC 6-55
CNF 6-56
COS 6-56
CRCAL? 6-57
CSCAL? 6-57
CSNUM 6-58
CSSLOT 6-58
CST 6-59
DBR 6-59
DRPFACT? 6-60
ERRSC 6-60
FBAND 6-61
FDN 6-61
FREQ 6-62
FREQADJ 6-63
FUP 6-63
FVECTERR? 6-64
HMODPWR? 6-64
INTPOL 6-65
JITTER? 6-65
KSA 6-66
KSG 6-66
KSH 6-67
LVLREL 6-67
M1 6-68
M2 6-68
MAGERR? 6-69
MAGTDERR? 6-69
MEANPWR? 6-70
MEAS 6-71
MEASOBJ 6-72
MKL? 6-73
MKN 6-73
MKOFF 6-74
MKP 6-74
MKR 6-75
MKRS 6-75
MKZ 6-76
MKZF 6-76
MODPWR? 6-77
MSTAT? 6-78
MTEMPREL 6-78
NUMSYM? 6-79
OBW? 6-79
OBWFREQ? 6-80
OCCBW? 6-80
OFF 6-81
OFFPWR? 6-81
ORGNOFS? 6-82
PATT 6-82
PEAKPWR? 6-83
PHASEERR? 6-84
POWER? 6-84
PSSIOT 6-85
PVECTERR? 6-85
RAMPSYM? 6-86
RATIO? 6-86
RFATTN 6-87
RFLVL 6-87
RNG 6-88

TABLE OF CONTENTS (Continued)

RTNYQ 6-88
SAVETBL 6-89
SAVETEMP 6-89
SCAL 6-90
SCNCT 6-90
SCOFS 6-91
SETREL 6-91
SLCTTBL 6-92
SLCTTEMP 6-92
SLOTPWR? 6-93
SPUFREQ 6-94
SPUHRM 6-95
SPULVL? 6-95
STARTPT 6-96
STD27 6-96
STORAGE 6-97
SWPWR? 6-98
SYMTIME 6-99
SYS 6-99
TEMPLVL 6-100
TERM 6-101
TIMING? 6-101
TXPWR? 6-102
TXTIME 6-102
UCAL 6-103
UNIT 6-104
UNT 6-105
VAVG 6-106
VECTERR? 6-106
WINDOW 6-107
ZAJ 6-107
ZEROSET 6-108

6.4 Spectrum mode commands 6-110
AAT 6-111
AMD 6-111
ARB 6-112
AST 6-112
ASWT 6-113
AT 6-113
ATT 6-114
ATUN 6-114
AUNITS 6-115
AUTO 6-115
AVB 6-116
AVR 6-116
AWR 6-117
A1 6-117
A2 6-118
BNDC 6-118
BSAUTO 6-119
CA 6-119
CAL 6-120
CF 6-120
CLRW 6-121
CMK? 6-121
CNF 6-122
COUPLE 6-122
CR 6-123
CT 6-123
CV 6-124
DET 6-124
DETM 6-125
DFMT 6-125
DPOINT 6-126
EXTTYPE 6-126
E1 6-127
E2 6-127
E3 6-128
E4 6-128
FA 6-129
FB 6-129
FDN 6-130
FMRNG 6-130
FRQ 6-131
FS 6-131
FSS 6-132
FUP 6-132
GATE 6-133
GD 6-133
GE 6-134
GL 6-134
HN 6-135
HNLOCK 6-135
HNUNLK 6-136
KSA 6-136
KSB 6-137
KSC 6-137

TABLE OF CONTENTS (Continued)

KSD 6-138
KSG 6-138
KSH 6-139
KSO 6-139
LG 6-140
LN 6-140
LSS 6-141
LSSA 6-141
MKA? 6-142
MKACT 6-142
MKCF 6-143
MKD 6-143
MKF? 6-144
MKL? 6-144
MKLIST 6-145
MKMCL 6-145
MKMHI 6-146
MKMHRM 6-146
MKMIN 6-147
MKML? 6-147
MKMP 6-148
MKMULTI 6-148
MKN 6-149
MKOFF 6-149
MKP 6-150
MKPK 6-150
MKR 6-151
MKRL 6-151
MKS 6-152
MKSLCT 6-152
MKSP 6-153
MKSS 6-153
MKTRACK 6-154
MKW 6-154
MKZ 6-155
MKZF 6-155
MON 6-156
MONVOL 6-156
MT0 6-157
MT1 6-157
MXMH 6-158
MZW 6-158
MZWF 6-159
M1 6-159
M2 6-160
M3 6-160
PARAM 6-161
PCF 6-161
PP 6-162
PRESEL 6-162
PRL 6-163
PSW 6-163
RB 6-164
RBW 6-164
RL 6-165
RLV 6-166
RMK? 6-166
SCL 6-167
SOF 6-167
SP 6-168
SPD 6-168
SPF 6-169
SPFUNC 6-169
SPU 6-170
SS 6-170
ST 6-171
STF 6-171
SWT 6-172
TDLY 6-172
TEXPAND 6-173
TM 6-173
TMMD 6-174
TMWR 6-174
TRG 6-175
TRGLVL 6-175
TRGS 6-176
TRGSLP 6-176
TRGSOURCE 6-177
TS 6-177
TSP 6-178
TVLINE 6-178
TVSFRM 6-179
TVSTND 6-179
TZONE 6-180
TZSP 6-180
TZSTART 6-181
UCL? 6-181
UNC 6-182

TABLE OF CONTENTS (Continued)

UNT 6-182
VAVG 6-183
VB 6-183
VBCOUPLE 6-184
VBR 6-184
VBW 6-185
VIEW 6-185

(Blank)

6.1 IEEE 488.2 common commands

*CLS

*CLS Clear Status Command

■ Function Clears the Status Byte Register.

Header	Program command	Query	Response
*CLS	*CLS	———	———

■ Example *CLS

---

*ESE

*ESE Standard Event Status Enable

■ Function Sets or clears the Standard Status Enable Register.

Header	Program command	Query	Response
*ESE	*ESE␣n	*ESE?	n

■ Value of n 0 to 255

■ Example *ESE␣20
*ESE?

*ESR? Standard Event Status Register Query

■ Function Returns the current value in the Standard Event Status Register.

Header	Program command	Query	Response
*ESR?	———	*ESR?	n

■ Value of n 0 to 255

■ Example *ESR?

*IDN? Identification Query

■ Function Returns the manufacturer name, model number etc. of the product.

Header	Program command	Query	Response
*IDN?	———	*IDN?	ANRITSU,MS8604A,0,n

■ Value of n 1 to 99 (firmware version No.)

■ Example *IDN?

*OPC

*OPC Operation Complete Command

■ Function

Sets the bit 0 digit in the Standard Event Status Register when all pending selected device operations have been completed.

Header	Program command	Query	Response
*OPC	*OPC	———	———

■ Example

*OPC

*OPC?

*OPC? Operation Complete Query

■ Function

Sets 1 in the Output Queue to generate an MAV summary message when all pending selected device operations have been completed.

Header	Program command	Query	Response
*OPC?	———	*OPC?	1

■ Example

*OPC?

* PCB Pass Control Back

■ Function Passes the bus control authority.

Header	Program command	Query	Response
*PCB	*PCB␣a	———	———

■ Value of a 0 to 30

■ Example *PCB␣Ø

* PSC Power on Status Clear

■ Function Sets or clears the power on status clear flag.

Header	Program command	Query	Response
*PSC	*PSC␣n	*PSC?	n

■ Value of n 0, 1

■ Example *PSC␣Ø
*PSC?

*PSC?

*PSC? Power on Status Clear Query

■ Function Returns the current value of the power on status clear flag.

Header	Program command	Query	Response
*PSC?	———	*PSC?	n

■ Value of n 0, 1

■ Example *PSC?

---

*RST

*RST Reset Command

■ Function Resets the device in the third level.

Header	Program command	Query	Response
*RST	*RST	———	———

■ Example *RST

*SRE Service Request Enable Command

■ Function Sets the bits in the Service Request Enable Register.

Header	Program command	Query	Response
*SRE	*SRE	*SRE?	n

■ Value of n 0 to 63, 128 to 191 (current value of Service Request Enable Register)

■ Example *SRE

*STB? Read Status Byte Command

■ Function Returns the current values of the status bytes including the MSS bit.

Header	Program command	Query	Response
*STB?	———	*STB?	n

■ Value of n

Bit	Bit weight	Bit name	Conditions of Status Byte Register
7	128	——	0 = Not used
6	64	MSS	0 = Service not requested, 1 = Service requested
5	32	ESB	0 = Event status not generated, 1 = Event status generated
4	16	MAV	0 = No data in Output Queue, 1 = Data in Output Queue
3	8	——	0 = Not used
2	4	ESB(END)	0 = Event status not generated, 1 = Event status generated
1	2	ESB(PTA)	0 = Event status not generated, 1 = Event status generated
0	1	——	0 = Not used

■ Example *STB?

*TRG

*TRG Trigger Command

■ Function

Same function as that of IEEE488.1 GET-Group Execute Trigger-bus command. For this command, the MS8604A executes a single sweep (same function as SWP.)

Header	Program command	Query	Response
*TRG	*TRG	———	

■ Example

*TRG

*TST?

*TST? Self Test Query

■ Function

Executes a self-test and returns the results of any errors.

Header	Program command	Query	Response
*TST?	———	*TST?	n

■ Value of n

Ø: Indicates that the self-test completed without errors.

−32767 to −1, 1 to 32767: Indicates that the self-test did not complete, or completed with errors.

■ Example

*TST?

*WAI Wait-to-Continue Command

■ Function Keeps the next command on stand-by while the device is executing a command.

Header	Program command	Query	Response
*WAI	*WAI	———	

■ Example *WAI

6.2 MS8604A common commands

ALARM Alarm

■ Function Turns the alarm on and off.

Header	Program command	Query	Response
ALARM	ALARM␣a	ALARM?	a

■ Value of a
ON: Turns the alarm ON and buzzes the alarm once.
OFF: Turns the alarm OFF.

■ Suffix code None

■ Initial setting OFF

■ Example ALARM␣ON

BAUD Baud Rate (valid only when option 02 RS-232C is used)

■ Function Sets the Baud rate of the RS-232C.

Header	Program command	Query	Response
BAUD	BAUD␣a	BAUD?	a

■ Value of a 9600, 4800, 2400, 1200, 600, 300,

■ Suffix code None

■ Initial setting 2400

■ Example BAUD␣9800

BEP

BEP Buzzer Switch

■ Function Turns the buzzer switch ON or OFF (whether to buzz when an error occurs).

Header	Program command	Query	Response
BEP	BEP␣sw sw=ON, 1, OFF, 0	———	———

■ Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code None

■ Initial setting ON: ON

■ Example
```
BEP␣ON
```

BIN

BIN ASCII/Binary Data Out

■ Function Outputs the trace data in ASCII or BINARY format.

Header	Program command	Query	Response
BIN	BIN␣a a=0, 1, ON, OFF	———	———

■ Value of a
Ø: ASCII
1: BINARY
OFF: ASCII
ON: BINARY

■ Suffix code None

■ Initial setting Ø: ASCII

■ Example
```
BIN␣Ø
BIN␣ON
```

BZR Sounds Buzzer

■ Function Sounds the buzzer.

Header	Program command	Query	Response
BZR	BZR	———	———

■ Example BZR

CONTS Continuous Sweep Mode

■ Function Sets the sweep mode to continuous mode (same function as S1).

Header	Program command	Query	Response
CONTS	CONTS	———	———

■ Example CONTS

DATE

DATE Date

■ Function Sets the clock built in MS8604A instrument to the specified date.

Header	Program command	Query	Response
DATE	DATE␣yy,mm,dd	DATE?	yy,mm,dd

■ Value of yy 00 to 99 (year)
■ Value of mm 01 to 12 (month)
■ Value of dd 01 to 31 (day)
■ Suffix code None
■ Example DATE␣92,Ø8,31

DSPL

DSPL Display

■ Function Turns the screen display on and off.

Header	Program command	Query	Response
DSPL	DSPL␣a	DSPL?	a

■ Value of a
ON: On Displays the screen.
OFF: Off Does not display the screen.
■ Suffix code None
■ Initial setting ON
■ Example DSPL␣OFF

DTAB Data Bit (valid only when option 02 RS-232C is used)

■ Function Sets the data bit of the RS-232C.

Header	Program command	Query	Response
DTAB	DTAB␣a	DTAB?	a

■ Value of a
7: 7 bit
8: 8 bit

■ Suffix code None

■ Initial setting 8

■ Example DTAB␣7

ESE1 Event Status Enable (PTA)

■ Function Allows the PTA Event Status Enable Register to select which bit in the corresponding Event Register causes a TRUE ESB summary message bit 1 when set.

Header	Program command	Query	Response
ESE1	ESE1␣a a = 0 to 255	ESE1?	a a = 0 to 255

■ Value of a
0 to 255:
Represents the sum of the bit weighted values enabled by the square of the bit number corresponding to bits 0, 1, 2, 3, 4, 5, 6, 7 of END Event Status Register.

■ Suffix code None

■ Example ESE1␣1

ESE2

ESE2 Event Status Enable (END)

■ Function

Allows the END Event Status Enable Register to select which bit in the corresponding Event Register causes a TRUE ESB summary message bit 2 when set.

Header	Program command	Query	Response
ESE2	ESE2␣a a = 0 to 255	ESE2?	a a = 0 to 255

■ Value of a

0 to 255:
Represents the sum of the bit weighted values enabled by the square of the bit number corresponding to bits 0, 1, 2, 3, 4, 5, 6, 7 of END Event Status Register.

■ Suffix code

None

■ Example

ESE2␣1

ESR1?

ESR1? Event Status Register (PTA)

■ Function

Allows the sum of the binary-weighted event bit values of the PTA Event Status Register to be read out by converting them to decimals. After readout, the PTA Event Status Register is reset to 0.

Header	Program command	Query	Response
ESR1?	———	ESR1?	a a = 0 to 255

■ Value of a

0 to 255

■ Suffix code

None

■ Example

ESR1?

ESR2? Event Status Register (END)

■ Function

Allows the sum of the binary-weighted event bit values of the END Event Status Register to be read out by converting them to decimals. After readout, the END Event Status Register is reset to 0.

Header	Program command	Query	Response
ESR2?	———	ESR2?	a a = 0 to 255

■ Value of a 0 to 255

■ Suffix code None

■ Example ESR2?

GPIA GPIB 2 Self Address

■ Function

Sets GPIB 2 self address.

Header	Program command	Query	Response
GPIA	GPIA␣a a=0 to 30	GPIA?	a a=0 to 30

■ Value of a 0 to 30

■ Suffix code None

■ Initial setting Value of a = 16 (provided the address already allocated is not initialized)

■ Example
```
GPIA␣Ø
GPIA␣3Ø
```

GTOUT

GTOUT GPIB Time Out

■ Function Sets the time-out time of the GPIB.

Header	Program command	Query	Response
GTOUT	GTOUT␣a	GTOUT?	a

■ Value of a 0 to 255 (seconds, 1-second steps)

■ Suffix code None

■ Initial setting Ø

■ Example GTOUT␣1ØØ

INI

INI Initialize

■ Function Initializes all measurement control parameters to be initialized (same function as PRE and IP).

Header	Program command	Query	Response
INI	INI	———	———

■ Example INI

IP Initialize

■ Function Initializes all measurement control parameters to be initialized (same function as PRE and INI).

Header	Program command	Query	Response
IP	IP	———	———

■ Example
```
IP
```


KSE Title Entry

■ Function Registers the title character string (same function as TITLE).

Header	Program command	Query	Response
KSE	KSE␣text	———	———

■ Value of text Character string within 32 characters enclosed by double quotation marks or single quotation marks

■ Example
```
KSE␣"MS8604A"
KSE␣'TX␣TESTER'
```

MC8104

MC8104 MC8104A Address

■ Function Set the GPIB address of the MC8104A.

Header	Program command	Query	Response
MC81Ø4	MC81Ø4␣a a=0 to 30	MC81Ø4?	a a=0 to 30

■ Value of a 0 to 30

■ Suffix code None

■ Initial setting Value of a=19 (provided the address already allocated is not initialized)

■ Example MC81Ø4␣2Ø

PLS

PLS Direct Plot Start

■ Function Starts direct plotting.

Header	Program command	Query	Response
PLS	PLS␣a a=0	———	———

■ Value of a Ø: PLOT START

■ Suffix code None

■ Example PLS␣Ø

PMCS PMC Select

■ Function

Selects one from the PMC built in the MS8604A, external PMC in the MC8104A, or external floppy disk in the MC8104A.

Header	Program command	Query	Response
PMCS	PMCS␣a	PMCS?	a a=IPMC, EPMC1 EPMC2, EFD

■ Value of a

IPMC: PMC built in this instrument
EPMC1: External PMC1
EPMC2: External PMC2
EFD: External FD

■ Suffix code

None

■ Initial setting

IPMC: PMC built in this instrument

■ Example

```
PMCS␣IPMC
PMCS␣EFD
```


PMOD Printer Type

■ Function

Selects the type of printer for direct plotting.

Header	Program command	Query	Response
PMOD	PMOD␣a a=2 to 5	PMOD?	PMOD␣a

■ Value of a

2: Printer ····· ESC/P (8 dots)
3: Printer ····· HP2225 (HP)
4: Printer ····· MC8104A (Anritsu)
5: Video Plotter ····· UA455A
6: Printer ····· ESC/P (24 dots)

■ Suffix code

None

■ Initial setting

3: Printer ··· HP2225

■ Example

```
PMOD␣2
PMOD␣4
```

PNLMD

PNLMD Panel Mode

■ Function Sets the operation mode of the MS8604A.

Header	Program command	Query	Response
PNLMD	PNLMD␣a	PNLMD?	a

■ Value of a
TESTER: TX Test mode
SPECT: Spectrum mode
SYSTEM: System mode

■ Suffix code None

■ Initial setting TESTER

■ Example PNLMD␣SPECT

PRE

PRE Preset

■ Function Initializes all measurement control parameters which need to be initialized (same function as INI and IP).

Header	Program command	Query	Response
PRE	PRE	———	———

■ Example PRE

PRIA Direct Plot Printer Address

■ Function Sets the GPIB address of the printer for direct plotting.

Header	Program command	Query	Response
PRIA	PRIA␣a a=0 to 30	PRIA?	a a=0 to 30

■ Value of a 0 to 30

■ Suffix code None

■ Initial setting Value of a =17 (provided the address already allocated is not initialized)

■ Example PRIA␣17

PRINT Direct Plot Start

■ Function Starts direct plotting.

Header	Program command	Query	Response
PRINT	PRINT	———	———

■ Example PRINT

PRTY

PRTY Parity (valid only when option 02 RS-232C is used)

■ Function Sets the parity of the RS-232C.

Header	Program command	Query	Response
PRTY	PRTY␣a	PRTY?	a

■ Value of a
EVEN: Even number
ODD: Odd number
OFF: None

■ Suffix code None

■ Initial setting EVEN

■ Example PRTY␣ODD

RC

RC Recall Data from Internal Memory

■ Function Recalls trace data/parameter data from the built-in memory (same function as RGRC).

Header	Program command	Query	Response
RC	RC␣a a=1 to 4	———	———

■ Value of a 1 to 4 (memory No.)

■ Suffix code None

■ Example RC␣1

RCM Recall Data from PMC

■ Function Recalls measurement conditions (parameter) and trace (spectrum mode only) from PMC or floppy disk.

Header	Program command	Query	Response
RCM	RCM␣a a=1 to 99 101 to 199	———	———

■ Value of a 1 to 99 (File No. of spectrum mode)
101 to 199 (File No. of TX-Test mode)

■ Suffix code None

■ Example RCM␣17
RCM␣2

RDATA Recalled Data

■ Function Specifies the contents of data recalled.

Header	Program command	Query	Response
RDATA	RDATA␣a	RDATA?	a a=TP, P

■ Value of a TP: Trace & Parameter (spectrum mode only)
P: Parameter Only

■ Suffix code None

■ Initial setting TP: Trace & Parameter (provided the address already allocated is not initialized)

■ Example RDATA␣TP

RFINPUT

RFINPUT RF Input

■ Function Sets the RF input connector.

Header	Program command	Query	Response
RFINPUT	RFINPUT␣a	RFINPUT?	a

■ Value of a
HIGH: Input HIGH Power
LOW: Input LOW Power

■ Example RFINPUT␣HIGH

RGDIR

RGDIR Memory Directory

■ Function Displays the directory of recall memory.

Header	Program command	Query	Response
RGDIR	RGDIR	———	———

■ Example RGDIR

RGRC Recall Data from Internal Memory

■ Function Recalls trace data/parameter data from built-in memory (same function as RC).

Header	Program command	Query	Response
RGRC	RGRC␣a a=1 to 4	———	———

■ Value of a 1 to 4 (Memory No.)

■ Suffix code None

■ Example RGRC␣1

RGSV Save Data into Internal Memory

■ Function Saves trace data (spectrum mode only)/parameter data to built-in memory (same function as SV).

Header	Program command	Query	Response
RGSV	RGSV␣a a=1 to 4	———	———

■ Value of a 1 to 4 (Memory No.)

■ Suffix code None

■ Example RGSV␣1

SNGLS

SNGLS Single Sweep Mode

■ Function Sets the sweep to single (single sweep) mode (same function as S2).

Header	Program command	Query	Response
SNGLS	SNGLS	———	———

■ Example SNGLS

STPB

STPB Stop Bit (valid only when option 02 RS-232C is used)

■ Function Sets the stop bit of the RS-232C.

Header	Program command	Query	Response
STPB	STPB␣a	STPB?	a

■ Value of a
1: 1 bit
1.5: 1.5 bit
2: 2 bit

■ Suffix code None

■ Initial setting 1

■ Example STPB␣2

SV Save Data into Internal Memory

■ Function Saves trace data/parameter data to built-in memory (same function as RGSV).

Header	Program command	Query	Response
SV	SV␣a a=1 to 4	———	———

■ Value of a 1 to 4 (Memory No.)

■ Suffix code None

■ Example SV␣1

SVM Save Data into PMC

■ Function Saves the measurement conditions (parameter) and trace (spectrum mode only) to PMC or floppy disk.

Header	Program command	Query	Response
SVM	SVM␣s s=1 to 99 101 to 199	———	———

■ Value of s 1 to 99 (File No. of spectum mode)
101 to 199 (File No. of TX test mode)

■ Suffix code None

■ Example SVM␣17
SVM␣2

SWP

SWP — Single Sweep/Sweep Status

■ Function

Executes single sweep/Responds to sweep status (sweep completed/sweep in progress) When accepted by the MS8604A device, the SWP command causes a single sweep to be executed by setting the sweep mode to ' SINGLE '. The next command waits without being processed until its single sweep is completed (same function as TS). The SWP? Query command is used to Query the current sweep status (sweep completed/sweep in progress).

Header	Program command	Query	Response
SWP	SWP	SWP?	SWP␣a a=0,1

■ Value of a

Ø: Sweep completed
1: Sweep in progress

■ Example

```
SWP
SWP?
```

S1

S1 — Sweep Mode (Continuous)

■ Function

Sets the sweep mode to CONTINUOUS (same function as CONTS).

Header	Program command	Query	Response
S1	S1	———	———

■ Example

```
S1
```

S2 Sweep Mode (Single)

■ Function Sets the sweep mode to SINGLE (same function as SNGLS).

Header	Program command	Query	Response
S2	S2	———	———

■ Example S2

TIME Time

■ Function Sets the clock built in MS8604A instrument to the specified time.

Header	Program command	Query	Response
TIME	TIME␣hh,mm,ss	TIME?	hh,mm,ss

■ Value of hh 00 to 23 (hour)
■ Value of mm 00 to 59 (minute)
■ Value of ss 00 to 59 (second)
■ Suffix code None
■ Example TIME␣Ø8,3Ø,ØØ

TITLE

TITLE — Title Entry

■ Function — Registers the title character string (same function as KSE).

Header	Program command	Query	Response
TITLE	TITLE␣text	TITLE?	text

■ text — Character string within 32 characters enclosed by double quotation marks or single quotation marks

■ Example
```
TITLE␣"MS8604A"
TITLE␣'ANRITSU'
TITLE␣" "     (Title is not displayed.)
```

TOUT

TOUT — Time Out (valid only when option 02 RS-232C is valid)

■ Function — Sets the time-out time.

Header	Program command	Query	Response
TOUT	TOUT␣a	TOUT?	a

■ Value of a — 1 to 255 (seconds, 1-second steps)

■ Suffix code — None

■ Initial setting — 5

■ Example — TOUT␣1

TRM Terminator

■ Function Sets the terminator of the Response data transferred on the GPIB.

Header	Program command	Query	Response
TRM	TRM␣a a=0,1	———	———

■ Value of a
Ø: LF
1: CR/LF

■ Suffix code None

■ Initial setting Ø: LF (Provided the terminator already registered is not initialized)

■ Example
TRM␣Ø
TRM␣1

TTL Title Display Switch

■ Function Sets the title display mode to ON or OFF.

Header	Program command	Query	Response
TTL	TTL␣sw	TTL?	TTL␣sw

■ Value of sw
DATE: Date/Time
USER: User Define
ON: User Define
OFF: OFF

■ Suffix code None

■ Initial setting OFF: DATE

■ Example TTL␣ON

XMA

XMA Trace-FREQ Data

■ Function Writes/reads the spectrum trace data.

Header	Program command	Query	Response
XMA	XMA␣p,b	XMA␣p,d	b_1, b_2, b_3 ····· (When ASCII is specified) $b_1\ b_2\ b_3$ ····· (When BINARY is specified)

■ Value of p 0 to 1001 (point No. position)

■ Value of b LOG scale used:
Integers having 0.01 dBm unit (independent of display unit system)

LIN scale used: $b = \dfrac{\text{Voltage value (V)}}{\text{Reference level (V)}} \times 10000$

■ Value of d 1 to 1002 (number of points)

■ Initial setting
```
XMA␣1,-2000
XMA?␣1,2  (Reads out two data from point 1)
```

Note: When the binary format is specified for Response data, each point data is composed of two bytes, and each byte is sent out in sequence from the high-order byte to the low-order byte.

XMB

XMB OCC. BW/Adj. Ch. Data

■ Function Writes/reads the waveform data of the occupied frequency bandwidth (STANDARD) and adjacent channel leakage power (STANDARD).

Header	Program command	Query	Response
XMB	XMB␣p,b	XMB?␣p,d	b_1, b_2, b_3 ····· (When ASCII is specified) $b_1\ b_2\ b_3$ ····· (When BINARY is specified)

■ Value of p 0 to 1001 (point No. position)

■ Value of b Integers having 0.01 dBm unit (independent of display unit system)

■ Value of d 1 to 1002 (number of points)

■ Example
```
XMB␣1,-2000
XMB?␣1,2  (Reads out two data from point 1)
```

Note: When the binary format is specified for Response data, each point data is composed of two bytes, and each byte is sent out in sequence from the high-order byte to the low-order byte.

XMC Constellation Data

■ Function Writes/reads the constellation display data.

Header	Program command	Query	Response
XMC	XMC␣p0,p1,b	XMC␣p0,p1,d	b_1, b_2, b_3 ····· (When ASCII is specified) $b_1\ b_2\ b_3$ ····· (When BINARY is specified)

■ Value of p0 0: I Data
1: Q Data

■ Value of p1 0 to 648

■ Value of b Integers having 0.0001 dBm unit
−30000 to 30000

■ Value of d 1 to 649 (number of points)

■ Example
```
XMC␣1,2,-2000
XMC?␣0,1,2
```
(Reads out two data from point 1 of 1 data)

Note: When the binary format is specified for Response data, each point data is composed of two bytes, and each byte is sent out in sequence from the high-order byte to the low-order byte.

XMD RF Power Data

■ Function Writes/reads the power measurement data.

Header	Program command	Query	Response
XMD	XMD␣p,b	XMD?␣p,d	b_1, b_2, b_3 ····· (When ASCII is specified) $b_1\ b_2\ b_3$ ····· (When BINARY is specified)

■ Value of p 0 to 4560

■ Value of b Integers having 0.01 dBm unit (independent of display unit system)

■ Value of d 1 to 4561 (number of points)

■ Example
```
XMD␣1,-2000
XMD?␣1,2
```
(Reads out two data from point 1)

Note: When the binary format is specified for Response data, each point data is composed of two bytes, and each byte is sent out in sequence from the high-order byte to the low-order byte.

XME

XME Occ. BW. Data

■ Function — Writes/reads the waveform data of the occupied frequency bandwisth (HIGH SPEED).

Header	Program command	Query	Response
XME	XME␣p,b	XME␣p,d	b_1, b_2, b_3 ····· (When ASCII is specified) $b_1\, b_2\, b_3$ ····· (When BINARY is specified)

■ Value of p — 0 to 250 (point No. position)

■ Value of b — Integers having 0.01 dBm unit (independent of display unit system)

■ Value of d — 1 to 251 (number of points)

■ Example
```
XME␣1,-2000
XME?␣1,2 (Reads out two data from point 1)
```

Note: When the binary format is specified for Response data, each point data is composed of two bytes, and each byte is sent out in sequence from the high-order byte to the low-order byte.

XMT

XMT Trace-TIME Data

■ Function — Writes/reads the spectrum data to/from trace TIME memory.

Header	Program command	Query	Response
XMT	XMT␣p,b	XMT?␣p,d	b_1, b_2, b_3 ····· (When ASCII is specified) $b_1\, b_2\, b_3$ ····· (When BINARY is specified)

■ Value of p — 0 to 1001 (point No. position)

■ Value of b — LOG scale used:
Integers having 0.01 dBm unit (independent of display unit system)

LIN scale used: $b = \dfrac{\text{Voltage value (V)}}{\text{Reference level (V)}} \times 10000$

■ Value of d — 1 to 1002 (number of points)

■ Example
```
XMT␣1,-2000
XMT?␣1,2 (Reads out two data from point 1)
```

Note: When the binary format is specified for Response data, each point data is composed of two bytes, and each byte is sent out in sequence from the high-order byte to the low-order byte.

(Blank)

6.3 TX Test Commands

- Query command output format

  Measurement result responses other than the waveform memory are output in the following format:

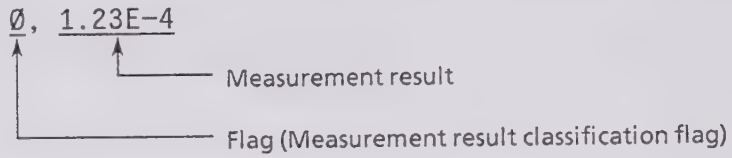

Flags have the following values depending on the result of the measurement:

Ø: Normal termination
1: Level over
2: Level under
8: No measurement result
9: Measurement abnormal termination

ADJCH? Adjacent Channel Power

■ Function

Outputs a measurement result on the adjacent channel leakage power measurement screen.

Header	Program command	Query	Response
ADJCH	————	ADJCH?␣a	c,d (Depends on display units.)
	————	ADJCH?␣a,b	c,d

■ Value of a

LOW3: Lower-3 (PDC: Invalid, PHS: Invalid, NADC: −90 kHz)
LOW2: Lower-2 (PDC: −100 kHz, PHS: −900 kHz, NADC: −60 kHz)
LOW1: Lower-1 (PDC: −50 kHz, PHS: −600 kHz, NADC: −30 kHz)
UP1 : Upper-1 (PDC: 50 kHz, PHS: 600 kHz, NADC: 30 kHz)
UP2 : Upper-2 (PDC: 100 kHz, PHS: 900 kHz, NADC: 60 kHz)
UP3 : Upper-3 (PDC: Invalid, PHS: Invalid, NADC: 90 kHz)

■ Value of b

DBM: dBm
WATT: mW, μW, nW
DB: dB

■ Value of c

Measurement result classification flag

■ Value of d

(dBm or dB value) −90 to 40.42
(output format: 0,*****)
(Watt value) 0.001 nW to 1000 mW
(output format: 0,*.**E+**)

■ Suffix code

None

■ Example

ADJCH?␣UP2,WATT

ADJMEAS

ADJMEAS Adjacent Channel Meas

■ Function

Sets the Meas function on the adjacent channel leakage power measurement screen.

Header	Program command	Query	Response
ADJMEAS	ADJMEAS␣a	ADJMEAS?	a

■ Value of a OFF, ON

■ Example ADJMEAS␣ON

AUNITS

AUNITS Unit for Log Scale

■ Function

Sets one of the display unit systems when the LOG scale is selected.

Header	Program command	Query	Response
AUNITS	AUNITS␣a	AUNITS?	a
	———	AUNITS?	b

■ Value of a

DBM: dBm
Used for the power measurement, adjacent channel leakage power measurement or spurious measurement screen.

WATT: nW/μW/mW/W
Used for the power measurement screen.

■ Value of b

MW: mW
Used for the adjacent channel leakage power measurement or spurious measurement screen.

UW: μW
Used for the adjacent channel leakage power measurement or spurious measurement screen.

NW: nW
Used for the adjacent channel leakage power measurement or spurious measurement screen.

DB: dB
Used for the adjacent channel leakage power measurement or spurious measurement screen.

■ Suffix code None

■ Initial setting DBM: dBm

AUTORNG Auto Range

■ Function

Executes Auto Range of Calibration on modulation analysis, power measurement, occupied bandwidth measurement, adjacent channel leakage power measurement, or spurious measurement screen.

Header	Program command	Query	Response
AUTORNG	AUTORNG	AUTORNG?	a

■ Value of a

Before execution of Auto range: RF level value on the parameter setting screen
After execution of Auto range: RF level value obtained by the measuring instrument

■ Suffix code None

■ Initial setting None

■ Example AUTORNG

AVR Average Number

■ Function

Sets the mean processing count on the power measurement, occupied bandwidth measurement, or adjacent channel leakage power measurement screen.

Header	Program command	Query	Response
AVR	AVR␣a	AVR?	a
	———	AVR?␣RFPWR (Use this query when reading Average No. of the power measurement screen from a screen other then the power measurement screen.)	a
	———	AVR?␣OBW (Use this query to read Average No. of the occupied bandwidth measurement screen from a screen other than the occupied bandwidth measurement screen.)	a
	———	AVR?␣ADJ (Use this query to read Average No. of the adjacent channel leakage power measurement screen from a screen other than the adjacent channel leakage power measurement screen.)	a

■ Value of a 2 to 99 (integer steps)

■ Suffix code None

■ Initial setting 4

■ Example AVR␣32

BITR?

BITR? Bit Rate

■ Function

Outputs the bit rate of the measurement result on the modulation analysis screen.

Header	Program command	Query	Response
BITR	———	BITR?	a,b

■ Value of a — Measurement result classification flag

■ Value of b — 0 to 9 999.999 999 9 kbps (0.000 000 1 steps)

■ Suffix code — None

■ Example — BITR?

BITRERR?

BITRERR? Bit Rate Error

■ Function

Outputs the bit rate error of a measurement result on the modulation analysis screen.

Header	Program command	Query	Response
BITRERR	———	BITRERR?	a,b

■ Value of a — Measurement result classification flag

■ Value of b — −500.0 to 500.0 ppm (0.1 steps)

■ Suffix code — None

■ Example — BITRERR?

BPATT Bit Pattern

■ Function Sets the USER bit pattern of SYNC (UNIQUE) WORD on the parameter setting screen.

Header	Program command	Query	Response
BPATT	BPATT␣a	BPATT?	a

■ Value of a 0--0 to 1--1

■ Suffix code None

■ Initial setting ----

■ Example BPATT␣10010011

BS Back Screen

■ Function Returns to the upper level of the screen.

Header	Program command	Query	Response
BS	BS	———	———

■ Example BS

BSTAVG

BSTAVG 10 Burst Average

■ Function Sets 10 Burst Average on the modulation analysis screen.

Header	Program command	Query	Response
BSTAVG	BSTAVG␣a	BSTAVG?	a

■ Value of a
ON: On
OFF: Off

■ Suffix code None

■ Initial setting OFF

■ Example BSTAVG␣ON

CALADJ

CALADJ Cal. Adjust

■ Function Executes Cal.Adjust on the parameter screen.

Header	Program command	Query	Response
CALADJ	CALADJ	———	———

■ Suffix code None

■ Initial setting None

■ Example CALADJ

CALOSC Cal. Oscillator

■ Function Sets Cal.Oscillator on the parameter screen.

Header	Program command	Query	Response
CALOSC	CALOSC␣a	CALOSC?	a

■ Value of a
ON: On
OFF: Off

■ Suffix code None

■ Initial setting OFF

■ Example CALOSC␣ON

CARRF? Carrier Frequency

■ Function Outputs the carrier frequency of a measurement result on the modulation analysis screen.

Header	Program command	Query	Response
CARRF	———	CARRF?	a,f f= 100 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of a Measurement result classification flag

■ Value of f 100 Hz to 8.5 GHz

■ Suffix code None

■ Initial setting None

■ Example CARRF?

CARRFERR?

CARRFERR? Carrier Frequency Error

■ Function Outputs the carrier frequency error of a measurement result on the modulation analysis, or constellation screen.

Header	Program command	Query	Response
CARRFERR	———	CARRFERR?	a,f f= −999999.9 to 0 to 999999.9 Transfers the data without suffix code as if represented in units of Hz

■ Value of a Measurement result classification flag

■ Value of f −999.999 9 kHz to 999.999 9 kHz (0.1 Hz steps)

■ Suffix code None

■ Example CARRFERR?

CDJ

CDJ Cal. Adjust

■ Function Executes Cal.Adjust on the power meter screen (same function as CALADJ).

Header	Program command	Query	Response
CDJ	CDJ	———	———

■ Suffix code None

■ Initial setting None

■ Example CDJ

CF Center Frequency

■ Function — Sets the FREQUENCY frequency on the parameter setting screen and the frequency on the power meter screen (same function as FREQ).

Header	Program command	Query	Response
CF	CF␣f CF␣a	CF?	f f=100 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f — 100 Hz to 8.5 GHz

■ Value of a — UP: CENTER FREQ STEP UP (Same function as FUP)
DN: CENTER FREQ STEP DOWN (Same function as FDN)

■ Suffix code — f: None: Hz
HZ: Hz
KHZ, KZ: kHz
MHZ, MZ: MHz
GHZ, GZ: GHz

a: None

■ Initial setting — Value of f = 940.025 MHz (PDC), 1895.15 MHz (PHS), 825.03 MHz (NADC), 1 GHz (power meter screen)

■ Example
```
CF␣1235456
CF␣50MHz
CF␣UP
```


CHAN Channel

■ Function — Sets the channel of FREQUENCY on the parameter setting screen.

Header	Program command	Query	Response
CHAN	CHAN␣a CHAN␣b	CHAN?	a

■ Value of a — Ø to 9999

■ Value of b — UP: step up
DN: step down

■ Suffix code — None

■ Initial setting — 1Ø01 (PDC, PHS), 1 (NADC)

■ Example
```
CHAN␣1Ø05
```

CHCARR

CHCARR Channels per Carrier

■ Function Sets the channels per carrier of SIGNAL on the parameter setting screen.

Header	Program command	Query	Response
CHCARR	CHCARR␣a	CHCARR?	a

■ Value of a
FULL: 3 (FULL RATE)
HALF: 6 (HALF RATE)

■ Suffix code None

■ Initial setting FULL (PDC, NADC)

■ Example CHCARR␣HALF

CHFREQ

CHFREQ Ch & Freq

■ Function Sets the Ch & Freq of FREQUENCY on the parameter setting screen.

Header	Program command	Query	Response
CHFREQ	CHFREQ␣a, f	———	———

■ Value of a Ø to 9999

■ Value of f 100 Hz to 8.5 GHz

■ Suffix code
None: Hz
HZ: Hz
KHZ, KZ: kHz
MHZ, MZ: MHz
GHZ, GZ: GHz

■ Initial setting 1001 channels, 940.025 MHz (PDC), 1895.15 MHz (PHS)
1 channel, 825.03 MHz (NADC)

■ Example CHFREQ␣1ØØ5, 8ØØMHZ

CHNUM Ch & Freq

■ Function Sets the Ch & Freq of FREQUENCY on the parameter setting screen of NADC.

Header	Program command	Query	Response
CHNUM	CHNUM␣a	———	———

■ Value of a 1 to 799, 990 to 1023

■ Suffix code
None: Hz
HZ: Hz
KHZ, KZ: kHz
MHZ, MZ: MHz
GHZ, GZ: GHz

■ Initial setting 1 channel, 825.03 MHz (NADC)

■ Example CHNUM␣1Ø05

CHSPC Channel Spacing

■ Function Sets the Channel Spacing of SIGNAL on the parameter setting screen.

Header	Program command	Query	Response
CHSPC	CHSPC␣f	CHSPC?	f f=1 to 1000000 Transfer the data without suffix code as if represented in units of Hz

■ Value of f 1 Hz to 1 MHz

■ Suffix code
None: Hz
HZ: Hz
KHZ, KZ: kHz
MHZ, MZ: MHz
GHZ, GZ: GHz

■ Initial setting 25 kHz (PDC), 300 kHz (PHS), 30 kHz (NADC)

■ Example CHSPC␣12.5KHZ

CNF

CNF Center Frequency

■ Function

Sets the FREQUENCY frequency on the parameter setting screen and the frequency on the power meter screen.

Header	Program command	Query	Response
CNF	CNF␣f	CNF?	CNF␣f f=100 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f

100 Hz to 8.5 GHz

■ Suffix code

None: Hz
HZ: Hz
KHZ, KZ: kHz
MHZ, MZ: MHz
GHZ, GZ: GHz

■ Initial setting

940.025 MHz (PDC), 1895.15 MHz (PHS), 825.03 MHz (NADC), 1 GHz (power meter screen)

■ Example

```
CNF␣123456
CNF␣5ØMHZ
CNF?
```

COS

COS Cal. Oscillator Start

■ Function

Turns on Cal.Oscillator on the power meter screen (same function as CALOSC ON).

Header	Program command	Query	Response
COS	COS	———	———

■ Suffix code

None

■ Initial setting

None

■ Example

```
COS
```

CRCAL? Raference Cal Facter

■ Function Outputs the Reference Cal Factor on the power meter screen.

Header	Program command	Query	Response
CRCAL	———	CRCAL?	a

■ Value of a −2.00 dB to 2.00 dB

■ Example CRCAL?

CSCAL? Sensor Cal Facter

■ Function Outputs the Sensor Cal factor on the power meter.

Header	Program command	Query	Response
CSCAL	———	CSCAL?	a

■ Value of a −2.00 dB to 2.00 dB

■ Example CSCAL?

CSNUM

CSNUM CS Slot Number Active

■ Function Sets the CS Slot Number Active on the parameter setting screen.

Header	Program command	Query	Response
CSNUM	CSNUM␣a	CSNUM?	a

■ Value of a 1 to 4

■ Example CSNUM␣2

CSSLOT

CSSLOT CS Slot Number

■ Function Sets the CS Slot Number on the parameter setting screen.

Header	Program command	Query	Response
CSSLOT	CSSLOT␣a,b	CSSLOT?␣a	b

■ Value of a 1 to 4

■ Value of b OFF, ON

■ Example CSSLOT␣2,ON

CST Cal. oscillator Stop

■ Function Turns off Cal.Oscillator on the parameter screen (same function as CALOSC OFF).

Header	Program command	Query	Response
CST	CST	———	———

■ Suffix code None
■ Initial setting None
■ Example CST

DBR dB Relative

■ Function Sets the relative mode on the power meter screen (same function as SETREL).

Header	Program command	Query	Response
DBR	DBR	———	———

■ Suffix code None
■ Initial setting None
■ Example DBR

DRPFACT?

DRPFACT? Droop Factor

■ Function — Outputs the droop factor of a measurement result on the modulation analysis screen.

Header	Program command	Query	Response
DRPFACT	———	DRPFACT?	a,b

■ Value of a — Measurement result classification flag

■ Value of b — −3.2768 to 3.2767 dB/symbol (0.0001 steps)

■ Suffix code — None

■ Example — DRPFACT?

ERRSC

ERRSC Error Scale

■ Function — Sets the error scale of the constellation display screen.

Header	Program command	Query	Response
ERRSC	ERRSC␣a	ERRSC?	a

■ Value of a
5: 5 %
1Ø: 10 %
2Ø: 20 %
OFF: Off

■ Suffix code — None

■ Initial setting — OFF

■ Example — ERRSC␣2Ø

FBAND Frequency Band

■ Function Sets the Frequency Band on the parameter setting screen.

Header	Program command	Query	Response
FBAND	FBAND␣f	FBAND?	f

■ Value of f 800, 1500

■ Suffix code MHz, MZ: MHz

■ Example FBAND␣8ØØMHz

FDN Frequency Step Down

■ Function Decreases the FREQUENCY frequency on the parameter setting screen and frequency on the power meter screen by the steps set by the frequency step size. (same function as FREQ␣DN).

Header	Program command	Query	Response
FDN	FDN	———	———

■ Example FDN

FREQ

FREQ Frequency

■ Function

Sets the FREQUENCY frequency on the parameter setting screen and the frequency on the power meter screen.

Header	Program command	Query	Response
FREQ	FREQ␣f FREQ␣a ———	FREQ? (Use this query on the current screen.) ——— FREQ?␣PWRMTR (Use this query when reading the frequency set on the power meter screen from a screen other than the power meter screen.)	f f=100 to 8500000000 Transfers the data without suffix code sd if represented in units of Hz f

■ Value of f

100 Hz to 8.5 GHz

■ Value of a

UP: step up
DN: step down

■ Suffix code

None: Hz
HZ: Hz
KHZ, KZ: kHz
MHZ, MZ: MHz
GHZ, GZ: GHz

■ Initial setting

940.025 MHz (PDC), 1895.15 MHz (PHS), 825.03 MHz (NADC), 1 GHz (power meter screen)

■ Example

FREQ␣8ØØMHZ

FREQADJ Frequency Adjust

■ Function

Executes Frequency Adjust of Calibration on the modulation analysis, power measurement, occupied bandwidth measurement, adjacent channel leakage power measurement, or spurious measurement screen.

Header	Program command	Query	Response
FREQADJ	FREQADJ	FREQADJ?	f f= 100 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f

Before execution of Frequency adjust: Frequency value on parameter screen
After execution of Frequency adjust: Frequency value obtained by the measuring instrument

■ Suffix code None

■ Initial setting None

■ Example FREQADJ

FUP Frequency Step Up

■ Function

Increases the center frequency by the frequency step size, if it has been set (same function as FREQ_UP).

Header	Program command	Query	Response
FUP	FUP	———	———

■ Example FUP

FVECTERR?

FVECTERR? First 10 Symbol RMS Vector Error

■ Function Outputs the first 10 symbol RMS vector error of a measurement result on the modulation analysis screen.

Header	Program command	Query	Response
FVECTERR	———	FVECTERR?	a,b

■ Value of a Measurement result classification flag

■ Value of b −327.68 % to 327.67 % (rms) (0.01 % steps)

■ Suffix code None

■ Example FVECTERR?

HMODPWR?

HMODPWR? Modulation Power

■ Function Outputs the measurement result Modulation Power on the power measurement screen.

HMODPWR	———	HMODPWR?␣a	b,c

■ Value of a Omission: Units displayed on the screen
DBM: Units in dB (during REL display) or dBm (during ABS display)
WATT: Units in W

■ Value of b Measurement result classification flag

■ Value of c Outputs in units specified by value of a.

■ Example HMODPWR?

INTPOL Interpollation

■ Function Sets interpolation of the constellation display screen.

Header	Program command	Query	Response
INTPOL	INTPOL␣a	INTPOL?	a

■ Value of a
NON: Non Interpollation
LIN: Linear Interpollation
POINT4: 4-Points Interpollation

■ Suffix code None

■ Initial setting NON

■ Example INTPOL␣POINT4

JITTER? Jitter

■ Function Outputs the measurement result Jitter of the power measurement screen.

Header	Program command	Query	Response
JITTER	———	JITTER?␣a	b,c

■ Value of a
+: Jitter (+)
-: Jitter (−)

■ Value of b Measurement result classification flag

■ Value of c Outputs the measurement result by the bit units.

■ Example JITTER?␣+

KSA

KSA Unit for Log Scale

■ Function

Sets the unit system of LOG scale on the power measurement screen, adjacent channel leakage power measurement screen, and spurious measurement screen to dBm (same function as UNT_DBM).

Header	Program command	Query	Response
KSA	KSA	———	———

■ Example

```
KSA
```

KSG

KSG Average ON

■ Function

Allows the averaging to be used when set to ON.

Header	Program command	Query	Response
KSG	KSG	———	———

■ Example

```
KSG
```

KSH Average OFF

■ Function

Turns off the averaging processing on the power measurement screen, occupied bandwidth measurement screen, and adjacent channel leakage power measurement screen to set the mode for processing waveform to NORMAL.

Header	Program command	Query	Response
KSH	KSH	———	———

■ Example

```
KSH
```


LVLREL Level Relative

■ Function

Selects absolute or relative power on the power measurement screen.

Header	Program command	Query	Response
LVLREL	LVLREL␣a	LVLREL?	a

■ Value of a

OFF: Absolute power
ON: Relative power

■ Suffix code

None

■ Initial setting

ON

■ Example

```
LVLREL␣OFF
```

M1

M1 Marker Mode

■ Function Turns OFF the Marker Mode (same function as MKR_OFF).

Header	Program command	Query	Response
M1	M1	———	———

■ Example M1

M2

M2 Marker Mode

■ Function Sets the marker Mode to Normal (ON) mode (same function as MKR_NRM).

Header	Program command	Query	Response
M2	M2	———	———

■ Example M2

MAGERR? Magnitude Error

■ Function Outputs the magnitude error of a measurement result on the modulation analysis screen (same function as MAGTDERR).

Header	Program command	Query	Response
MAGERR	———	MAGERR?	a,b

■ Value of a Measurement result classification flag

■ Value of b −327.68 % to 327.67 % (rms) (0.01 % steps)

■ Suffix code None

■ Example MAGERR?

MAGTDERR? Magnitude Error

■ Function Outputs the magnitude error of a measurement result on the modulation analysis screen.

Header	Program command	Query	Response
MAGTDERR	———	MAGTDERR?	a,b

■ Value of a Measurement result classification flag

■ Value of b −327.68 % to 327.67 % (rms) (0.01 % steps)

■ Suffix code None

■ Initial setting None

■ Example MAGTDERR?

MEANPWR?

MEANPWR? Mean Power

■ Function

Outputs the mean power (PDC or PHS) of a measurement result on the adjacent channel leakage power measurement screen.

Header	Program command	Query	Response
MEANPWR?	———	MEANPWR?␣a	c,d (Depends on display units.)
	———	MEANPWR?␣a,b	c,d

■ Value of a

LOW2: Lower-2 (PDC: −100 kHz, PHS: −900 kHz)
LOW1: Lower-1 (PDC: −50 kHz, PHS: −600 kHz)
UP1: Upper-1 (PDC: 50 kHz, PHS: 600 kHz)
UP2: Upper-2 (PDC: 100 kHz, PHS: 900 kHz)

■ Value of b

DBM: dBm
WATT: mW, μW, nW
DB: dB

■ Value of c

Measurement result classification flag

■ Value of d

(dBm or dB value) −90 to 40.42
(output format: 0, *****)
(Watt value) 0.001 nW to 1000 mW
(output format: 0, *.**E+**)

■ Suffix code

None

■ Example

MEANPWR?␣UP2,WATT

MEAS Measurement

■ Function Sets the measurement screen.

Header	Program command	Query	Response
MEAS	MEAS␣a	MEAS?	a

■ Value of a

MODANAL:	Modulation analysis screen
CONSTEL:	Constellation screen
RFPWR:	Power measurement screen
SETTEMP:	Template setting screen
OBW,STD:	Occupied frequency bandwidth measurement screen (STANDARD)
OBW,SPECT:	Occupied frequency bandwidth measurement screen (SPECTRUM)
OBW,HIGH:	Occupied frequency bandwidth measurement screen (HIGH SPEED)
ADJ,STD1:	Adjacent channel leakage power measurement screen (STANDARD [ALL])
ADJ,STD2:	Adjacent channel leakage power measurement screen (STANDARD [SEPARATE])
ADJ,SPECT1:	Adjacent channel leakage power measurement screen (SPECTRUM [ALL])
ADJ,SPECT2:	Adjacent channel leakage power measurement screen (SPECTRUM [SEPARATE])
ADJ,HIGH:	Adjacent channel leakage power measurement screen (HIGH SPEED)
SPURIOUS,SPOT:	Spurious measurement screen (SPOT measurement)
SPURIOUS,SEARCH:	Spurious measurement screen (SEARCH measurement)
SETTABLE:	Spurious frequency setting screen
SCALTBL:	Sensor cal. factor setting screen

■ Example MEAS␣RFPWR

MEASOBJ Measuring Object

■ Function Sets the measuring object of SIGNAL on the parameter setting screen.

Header	Program command	Query	Response
MEASOBJ	MEASOBJ␣a	MEASOBJ?	a

■ Value of a

MSCONT:	MS-CONT	PDC only
MSCOM:	MS-COM	
MSSYNC:	MS-SYNC	
BSCONT:	BS-CONT	
BSCOM:	BS-COM	
BSSYNC:	BS-SYNC	
PSCONT:	PS-CONT	PHS only
PSCOM:	PS-COM	
CSCONT:	CS-CONT	
CSCOM:	CS-COM	
CONT:	CONTINUOUS	
MOBILE:	MOBILE	NADC only
SHORT:	SHORTENED BURST	
BASE:	BASE	

■ Suffix code None

■ Initial setting MS-COM (PDC), PS-COM (PHS), MOBILE (NADC)

■ Example MEASOBJ␣BSCONT

MKL? Marker Value

■ Function

Outputs the value of Marker on the modulation analysis screen and power measurement screen.

Header	Program command	Query	Response
MKL	———	MKL?	a

■ Value of a

Relative value (REL) display: Outputs the level of the marker value in dB.
Absolute value (ABS): Outputs the level of the marker value in dBm.
— power measurement screen

Outputs the level of the marker value in dBm.
— Adjacent channel leakage power measurement screen

■ Example

```
MKL?
```


MKN Marker or Maker Position

■ Function

Sets the Marker on the power measurement screen and adjacent channel leakage power measurement screen to NORMAL (same function as MKR␣NRM) or sets the Marker position (same function as MKRS).

Header	Program command	Query	Response
MKN	MKN	———	———
	MKN␣a	MKN?	(Sets to NORMAL.)
	MKN␣b		a (Sets the position.)

■ Value of a

Sets the marker position by the symbol or frequency.

■ Value of b

UP: Step UP
DN: Step DOWN

■ Example

```
MKN␣80.25
MKN␣UP
```

MKOFF

MKOFF Marker Mode

■ Function Turns off the marker mode.

Header	Program command	Query	Response
MKOFF	MKOFF␣a	———	———

■ Value of a
ALL: Marker off
None: Marker off

■ Suffix code None

■ Example
MKOFF␣ALL
MKOFF

MKP

MKP Marker Position

■ Function Sets the marker position on the power measurement screen and adjacent channel leakage power measurement screen.

Header	Program command	Query	Response
MKP	MKP␣a	MKP?	a

■ Value of a
0 to 360: power measurement screen
0 to 250: adjacent channel leakage power measurement screen

■ Example MKP␣200

MKR Marker

■ Function Sets the marker mode of the power measurement screen.

Header	Program command	Query	Response
MKR	MKR␣a	MKR?	b

■ Value of a
NRM: Normal
Ø: Normal
OFF: Off
2: Off

■ Value of b
NRM: Normal
OFF: Off

■ Suffix code None

■ Initial setting OFF

■ Example MKR␣NRM

MKRS Marker Position

■ Function Sets the Marker position on the power measurement screen and adjacent channel leakage power measurement screen (same function as MKN).

Header	Program command	Query	Response
MKRS	MKRS␣a MKRS␣b	MKRS? ———	a (Sets the position.)

■ Value of a Sets the marker position by the symbol or frequency.

■ Value of b
UP: Step UP
DN: Step DOWN

■ Example MKRS␣UP

MKZ

MKZ Marker Position

■ Function

Sets the Marker position on the power measurement screen and adjacent channel leakage power measurement screen (same function as MKP).

Header	Program command	Query	Response
MKZ	MKZ␣a	MKZ?	MKZ␣a

■ Value of a

0 to 360: power measurement screen
0 ~ 250: adjacent channel leakage power measurement screen

■ Example

MKZ␣200

MKZF

MKZF Marker Position

■ Function

Sets the Marker position on the power measurement screen and adjacent channel leakage power measurement screen

Header	Program command	Query	Response
MKZF	MKZF␣a	MKZF?	a

■ Value of a

Sets the marker position by the symbol or frequency.

■ Example

MKZF␣80.25

MODPWR? Mean Power due to Modulation

■ Function

Outputs the mean power due to modulation of a measurement result on the adjacent channel leakage power measurement screen.

Header	Program command	Query	Response
MODPWR	———	MODPWR?␣a	c,d (Depends on display units.)
	———	MODPWR?␣a,b	c,d

■ Value of a

LOW3:	Lower-3 (PDC:	Invalid,	PHS:	Invalid,	NADC: −90 kHz)
LOW2:	Lower-2 (PDC:	−100 kHz,	PHS:	−900 kHz,	NADC: −60 kHz)
LOW1:	Lower-1 (PDC:	−50 kHz,	PHS:	−600 kHz,	NADC: −30 kHz)
UP1:	Upper-1 (PDC:	50 kHz,	PHS:	600 kHz,	NADC: 30 kHz)
UP2:	Upper-2 (PDC:	100 kHz,	PHS:	900 kHz,	NADC: 60 kHz)
UP3:	Upper-3 (PDC:	Invalid,	PHS:	Invalid,	NADC: 90 kHz)

■ Value of b

DBM: dBm
WATT: mW, μW, nW
DB: dB

■ Value of c

Measurement result classification flag

■ Value of d

(dBm or dB value) −90 to 40.42
(output format: 0, *****)
(Watt value) 0.001 nW to 1000 mW
(output format: 0, *.**E+**)

■ Suffix code

None

■ Initial setting

None

■ Example

MODPWR?␣UP2,WATT

MSTAT?

MSTAT? Measurement Status

■ Function Reads measurement status error information.

Header	Program command	Query	Response
MSTAT	———	MSTAT?	a

■ Value of a
Ø: Normal termination
1: Level over (LEVEL OVER)
2: Level under (LEVEL UNDER)
3: Measurement unavailable (SIGNAL ABNORMAL)
4: Synchronous word detection unavailable (SYNC WORD NOT FOUND)
5: Power sensor abnormal (POWER SENSOR ABNORMAL)
6: An RF input exceeded the hardware limit (INPUT LEVEL OVER).
7: A spurious measurement frequency is not entered (SET FREQUENCY TABLE).

■ Suffix code None

■ Example MSTAT?

MTEMPREL

MTEMPREL Magnitude Template Relative

■ Function Selects absolute or relative power on the power measurement screen.

Header	Program command	Query	Response
MTEMPREL	MTEMPREL␣a	MTEMPREL?	a

■ Value of a
OFF: Absolute power
ON: Relative power

■ Suffix code None

■ Initial setting ON

■ Example MTEMPREL␣OFF

NUMSYM? Number of symbols

■ Function Outputs the number of analytical symbols on the parameter setting screen.

Header	Program command	Query	Response
NUMSYM?	———	NUMSYM?	a

■ Value of a Refer to "Panel Operation Part".

■ Suffix code None

■ Example NUMSYM?

OBW? Occupied Bandwidth

■ Function Outputs a measurement result on the occupied bandwidth measurement screen (same function as OCCBW?).

Header	Program command	Query	Response
OBW	———	OBW?	a , f Transfers the data without suffix code as if represented in units of Hz

■ Value of a Measurement result classification flag

■ Value of f 0.0 to 99.9 kHz (PDC), 0.0 to 999.9 kHz (PHS) ; 0.1 kHz steps

■ Suffix code None

■ Example OBW?

OBWFREQ?

OBWFREQ? Occupied Bandwidth Center Frequency

■ Function Outputs a measurement result on the occupied bandwidth measurement screen.

Header	Program command	Query	Response
OBWFREQ?	———	OBWFREQ? a	b,f Transfers the data without suffix code as if represented in units of Hz

■ Value of a
CENTER: Center frequency
LOWER: Lower frequency
Minus(−): Lower frequency
UPPER: Upper frequency
Plus(+): Upper frequency

■ Value of b Measurement result classification flag

■ Value of f −999.9 to 999.9 kHz (0.1 kHz steps)

■ Suffix code None

■ Example
OBWFREQ?␣CENTER
OBWFREQ?␣+

OCCBW?

OCCBW? Occupied Bandwidth

■ Function Outputs a measurement result on the occupied bandwidth measurement screen.

Header	Program command	Query	Response
OCCBW	———	OCCBW?	a,f Transfers the data without suffix code as if represented in units of Hz

■ Value of a Measurement result classification flag

■ Value of f 0.0 to 99.9 kHz (PDC), 0.0 to 999.9 kHz (PHS) ; 0.1 kHz steps

■ Suffix code None

■ Example OCCBW?

OFF Offset

■ Function Sets User Cal.Factor on the power meter screen (same function as that of UCAL).

Header	Program command	Query	Response
OFF	OFF␣a	———	———

■ Value of a −30.00 to 30.00 dB (0.01 steps)
■ Suffix code dB
■ Initial setting Ø
■ Example OFF␣3.Ø

OFFPWR? Carrier Off Power

■ Function Outputs the carrier off power of a measurement result on the power measurement screen.

Header	Program command	Query	Response
OFFPWR	———	OFFPWR?	a,b
	———	OFFPWR?␣DBM	a,c
	———	OFFPWR?␣WATT	a,d

■ Value of a Measurement result classification flag
■ Value of b Depends on the displayed units.
■ Value of c (dBm value) −70.46 to 40.42
(output format: 0, *****)
■ Value of d (Watt value) 0.1 nW to 10 W
(output format: 0, *.**E+**)
■ Suffix code None
■ Example OFFPWR?

ORGNOFS?

ORGNOFS? Origin Offset

■ Function — Outputs the origin offset of a measurement result on the modulation analysis screen.

Header	Program command	Query	Response
ORGNOFS	———	ORGNOFS?	a,b

■ Value of a — Measurement result classification flag

■ Value of b — −327.68 to 0 dB (0.01 steps)

■ Suffix code — None

■ Initial setting — None

■ Example — ORGNOFS?

PATT

PATT Pattern

■ Function — Sets a SYNC (UNIQUE) WORD pattern on the parameter setting screen.

Header	Program command	Query	Response
PATT	PATT␣a	PATT?	a

■ Value of a

S1 to S12:	S1 to S12	PDC only
SS1 to SS6:	SS1 to SS6	
B32:	32 bit	PHS only
B16:	16 bit	
SYNC1 to SYNC6:	Sync1 to Sync6	NADC only
NO:	NO	
USER:	USER	

■ Suffix code — None

■ Initial setting — S1 (PDC), 16 bit (PHS), Sync 1 (NADC)

■ Example — PATT␣USER

PEAKPWR? Peak Power

■ Function

Outputs the peak power (PDC or PHS) or mean power due to switching transients (NADC) of a measurement result on the adjacent channel leakage power measurement screen.

Header	Program command	Query	Response
PEAKPWR	———	PEAKPWR?␣a	c,d (Depends on display units.)
	———	PEAKPWR?␣a,b	c,d

■ Value of a

LOW3:	Lower-3 (PDC:	Invalid,	PHS:	Invalid,	NADC:	−90 kHz)
LOW2:	Lower-2 (PDC:	−100 kHz,	PHS:	−900 kHz,	NADC:	−60 kHz)
LOW1:	Lower-1 (PDC:	−50 kHz,	PHS:	−600 kHz,	NADC:	−30 kHz)
UP1:	Upper-1 (PDC:	50 kHz,	PHS:	600 kHz,	NADC:	30 kHz)
UP2:	Upper-2 (PDC:	100 kHz,	PHS:	900 kHz,	NADC:	60 kHz)
UP3:	Upper-3 (PDC:	Invalid,	PHS:	Invalid,	NADC:	90 kHz)

■ Value of b

DBM:	dBm
WATT:	mW, μW, nW
DB:	dB

■ Value of c

Measurement result classification flag

■ Value of d

(dBm or dB value)	−90 to 40.42 (output format: 0, *****)
(Watt value)	0.001 nW to 1000 mW (output format: 0, *.**E+**)

■ Suffix code

None

■ Example

```
PEAKPWR?␣UP2,WATT
```

PHASEERR?

PHASEERR? Phase Error

■ Function — Outputs the phase error of a measurement result on the modulation analysis screen.

Header	Program command	Query	Response
PHASEERR	———	PHASEERR?	a,b

■ Value of a — Measurement result classification flag

■ Value of b — −327.68 to 327.67 deg (rms) (0.01 steps)

■ Suffix code — None

■ Initial setting — None

■ Example — PHASEERR?

POWER?

POWER? Power

■ Function — Outputs a measurement result on the power meter screen.

Header	Program command	Query	Response
POWER	———	POWER?␣a	b,c

■ Value of a
DBM: Outputs a value in dBm.
WATT: Outputs a value in Watt.
DB: Outputs a value in dB.

■ Value of b — Measurement result classification flag

■ Value of c
(dBm or dB value) −30.00 to 40.42 (output format: 0, *****)
(Watt value) 1 μW to 10 W (output format: 0, *.**E+**)

■ Suffix code — None

■ Example — POWER?␣DB

PSSLOT PS Slot

■ Function Sets the PS Slot on the parameter setting screen.

Header	Program command	Query	Response
PSSLOT	PSSLOT␣a	PSSLOT?	a

■ Value of a OFF, ON

■ Example PSSLOT␣a

PVECTERR? Peak Vector Error

■ Function Outputs the peak vector error of a measurement result on the modulation analysis screen.

Header	Program command	Query	Response
PVECTERR	———	PVECTERR?	a,b

■ Value of a Measurement result classification flag

■ Value of b −327.68 % to 327.67 % (0.01 % steps)

■ Suffix code None

■ Example PVECTERR?

RAMPSYM?

RAMPSYM? Ramp up symbol point

■ Function Outputs a ramp up symbol point value on the parameter setting screen.

Header	Program command	Query	Response
RAMPSYM?	———	RAMPSYM?	a

■ Value of a Refer to "Panel Operation Part".

■ Suffix code None

■ Example RAMPSYM?

RATIO?

RATIO? On/Off Ratio

■ Function Outputs the on/off ratio of a measurement result on the power measurement screen.

Header	Program command	Query	Response
RATIO	———	RATIO?	a,b

■ Value of a Measurement result classification flag

■ Value of b −999.99 to 999.99 (0.1 steps)

■ Suffix code None

■ Example RATIO?

RFATTN RF Attenuater

■ Function Sets the RF Atten on the spurious measurement screen.

Header	Program command	Query	Response
RFATTN	RFATTN␣a	RFATTN?	a

■ Value of a
NRM: Normal
NOISE: Noise

■ Suffix code None

■ Initial setting NRM

■ Example RFATTN␣NOISE

RFLVL RF Level

■ Function Sets the RF level of INPUT on the parameter setting screen.

Header	Program command	Query	Response
RFLVL	RFLVL␣a RFLVL␣b	RFLVL?	a

■ Value of a −32 to 40

■ Value of b
UP: step up
DN: step down

■ Suffix code None

■ Initial setting 3Ø

■ Example RFLVL␣2Ø

RNG

RNG Range

■ Function Sets a measurement range on the power meter screen.

Header	Program command	Query	Response
RNG	RNG␣a RNGA (Automatic switching) RNG2 (0.1 mW hold) RNG3 (1 mW hold) RNG4 (10 mW hold) RNG5 (100 mW hold)	RNG? ——— ——— ——— ———	a ——— ——— ——— ———

■ Value of a
AUTO: Automatically switches the value.
HOLD: Holds the current status.

■ Suffix code None

■ Initial setting AUTO

■ Example RNG␣HOLD

RTNYQ

RTNYQ Root-Nyquist Filter

■ Function Sets the Root-Nyquist filter on the parameter setting screen.

Header	Program command	Query	Response
RTNYQ	RTNYQ␣a	RTNYQ?	a

■ Value of a
YES: Yes
ON: Yes ——— Program commands only
NO: No
OFF: No ——— Program commands only

■ Suffix code None

■ Initial setting YES

■ Example RTNYQ␣NO

SAVETBL Save Frequency Table

■ Function Sets the memory number in which the frequency table on the spurious frequency creation screen is saved.

Header	Program command	Query	Response
SAVETBL	SAVETBL␣a	———	———

■ Value of a
NO1: Memory No.1
NO2: Memory No.2
NO3: Memory No.3

■ Suffix code None

■ Initial setting NO1

■ Example SAVETBL␣NO3

SAVETEMP Save Template

■ Function Saves the template on the template creation screen.

Header	Program command	Query	Response
SAVETEMP	SAVETEMP␣a	———	———

■ Value of a
NO1: Saves the template in internal memory No.1.
NO2: Saves the template in internal memory No.2.
NO3: Saves the template in internal memory No.3.

■ Suffix code None

■ Initial setting None

■ Example SAVETEMP␣NO3

SCALT

SCALT Sensor Cal Table

■ Function Sets the Sensor Cal Table on the sensor cal. factor setting screen.

Header	Program command	Query	Response
SCALT	SCALT␣a,b	SCALT?␣a	b

■ Value of a Sets the table frequency.

■ Value of b Sets the sensor cal. factor value.

■ Suffix code
None: Hz
Hz: Hz
KHz,KZ: MHz
GHz,GZ: GHz

■ Example SCALT␣5ØMHz,Ø.Ø1

SCNCT

SCNCT Sensor Connect To

■ Function Sets the Sensor Connect To on the power meter screen.

Header	Program command	Query	Response
SCNCT	SCNCT␣a	SCNCT?	a

■ Value of a
TESTER: Connects the power sensor to the transmitter tester.
DUT: Connects the power sensor to a device to be measured.

■ Suffix code None

■ Initial setting TESTER

■ Example SCNCT␣DUT

SCOFS Error Scale Offset

■ Function Sets an error scale offset on the constellation screen.

Header	Program command	Query	Response
SCOFS	SCOFS␣a	SCOFS?	a

■ Value of a Ø: 0 degree
22.5: 22.5 degrees

■ Suffix code None

■ Initial setting Ø

■ Example SCOFS␣22.5

SETREL Set Relative

■ Function Sets the Relative mode of the power meter screen.

Header	Program command	Query	Response
SETREL	SETREL	———	———

■ Suffix code None

■ Initial setting None

■ Example SETREL

SLCTTBL

SLCTTBL Select Frequency Table

■ Function Sets the frequency table on the spurious measurement screen.

Header	Program command	Query	Response
SLCTTBL	SLCTTBL␣a	SLCTTBL?	a

■ Value of a
NO1: No.1 Frequency Table
NO2: No.2 Frequency Table
NO3: No.3 Frequency Table
NOT: Not selected ——— Responses only

■ Suffix code None

■ Initial setting NO1

■ Example SLCTTBL␣NO3

SLCTTEMP

SLCTTEMP Select Template

■ Function Sets the template of the power measurement screen.

Header	Program command	Query	Response
SLCTTEMP	SLCTTEMP␣a	SLCTTEMP?	a

■ Value of a
NO1: No.1
NO2: No.2
NO3: No.3
STD: Standard
OFF: Off
NOT: Not selected ——— Responses only

■ Suffix code None

■ Initial setting STD

■ Example SLCTTEMP␣NO3

SLOTPWR? Slot Mean Power

■ Function Outputs the Slot Mean Power on the power measurement screen.

Header	Program command	Query	Response
SLOTPWR	———	SLOTPWR?␣a	b,c (No CRT display)

■ Value of a 1 to 8

■ Value of b Measurement result classification flag

■ Value of c Outputs the measurement result in dBm units.

■ Example SLOTPWR?␣3

SPUFREQ

SPUFREQ Spurious Frequency

■ Function Sets the spurious frequency on the spurious frequency creation screen.

Header	Program command	Query	Response
SPUFREQ	SPUFREQ␣a,f SPUFREQ␣b	SPUFREQ?␣a ———	f f= 100 to 8500000000 Transfers the data without suffix code as if represented in units of Hz ———

■ Value of a F1 to F15

■ Value of f 100 Hz to 8.5 GHz
Ø: Cancels a setting.

■ Value of b HRM: Sets Harmonics.

■ Suffix code None

■ Initial setting

(Units: MHz)

	PDC	PHS	NADC
f1	1 880.050 000	3 790.300 000	1 650.060 000
f2	2 820.075 000	5 685.450 000	2 475.090 000
f3	3 760.100 000	7 580.600 000	3 300.120 000
f4	4 700.125 000	———	4 125.150 000
f5			5 950.180 000
f6			6 775.210 000
f7			7 600.240 000
f8			8 425.270 000
f9			9 250.300 000

■ Example
```
SPUFREQ␣F4,1.5GZ
SPUFREQ␣F5,Ø
```

SPUHRM Spurious Harmonics

■ Function Sets a higher harmonic frequency on the spurious frequency creation screen (same function as SPUFREQHRM).

Header	Program command	Query	Response
SPUHRM	SPUHRM	———	———

■ Suffix code None

■ Initial setting None

■ Example SPUHRM

SPULVL? Spurious Level

■ Function Outputs a measurement result on the spurious harmonics measurement screen.

Header	Program command	Query	Response
SPULVL	———	SPULVL?␣a	c,d (Depends on display units.)
	———	SPULVL?␣a,b	c,d

■ Value of a F1 to F15

■ Value of b
DBM : dBm
WATT: mW, μW, nW
DB : dB

■ Value of c Measurement result classification flag

■ Value of d
(dBm or dB value) −90 to 40.42 (output format: 0, *****)
(Watt value) 0.001 nW to 1000 mW (output format: 0, *.**E+**)

■ Suffix code None

■ Example SPULVL?␣F3

STARTPT

STARTPT Start Point

■ Function Sets the start point of SYNC (UNIQUE) WORD on the parameter setting screen.

Header	Program command	Query	Response
STARTPT	STARTPT␣a	STARTPT?	a

■ Value of a 2 to 140

■ Suffix code None

■ Initial setting 59 (PDC), 6 (PHS), 6 (NADC)

■ Example STARTPT␣34

STD27

STD27 RCR STD-27 Version

■ Function Sets the PDC RCR STD-27 version.

Header	Program command	Query	Response
STD27	STD27␣a	STD27?	a

■ Value of a B, C

■ Example STD27␣C

STORAGE Storage Mode

■ Function

Sets the storage mode of the power measurement, occupied bandwidth measurement, or adjacent channel leakage power measurement screen.

Header	Program command	Query	Response
STORAGE	STORAGE␣a	STORAGE?	a
	———	STORAGE?␣RFPWR (Use this query when reading the storage mode of the power measurement screen from a screen other than the power measurement screen.)	a
	———	STORAGE?␣OBW (Use this query when reading the storage mode of the occupied bandwidth measurement screen from a screen other than the occupied bandwidth measurement screen.)	a
	———	STORAGE?␣ADJ (Use this query when reading the storage mode of the adjacent channel leakage power measurement screen from a screen other than the adjacent channel leakage power measurement screen.)	a

■ Value of a

NRM: Normal
MAX: Max Hold (RF POWER only)
MIN: Min Hold (RF POWER only)
AVG: Average
CUM: Cumulative (RF POWER only)
OVER: Over-write (RF POWER only)
WIDE: Wide Dynamic Range (RF POWER only)

■ Suffix code None

■ Initial setting NRM

■ Example STORAGE␣MAX

SWPWR? Mean Power due to Switching Transients

■ Function

Outputs the mean power due to switching transients of a measurement result on the adjacent channel leakage power measurement screen of NADC.

Header	Program command	Query	Response
SWPWR	———	SWPWR?␣a	c,d (Depends on display units.)
	———	SWPWR?␣a,b	c,d

■ Value of a

LOW3: Lower-3 (PDC: Invalid, PHS: Invalid, NADC: −90 kHz)
LOW2: Lower-2 (PDC: −100 kHz, PHS: −900 kHz, NADC: −60 kHz)
LOW1: Lower-1 (PDC: −50 kHz, PHS: −600 kHz, NADC: −30 kHz)
UP1: Upper-1 (PDC: 50 kHz, PHS: 600 kHz, NADC: 30 kHz)
UP2: Upper-2 (PDC: 100 kHz, PHS: 900 kHz, NADC: 60 kHz)
UP3: Upper-3 (PDC: Invalid, PHS: Invalid, NADC: 90 kHz)

■ Value of b

DBM: dBm
WATT: mW, μW, nW
DB: dB

■ Value of c

Measurement result classification flag

■ Value of d

(dBm or dB value) −90 to 40.42
(output format: 0, *****)
(Watt value) 0.001 nW to 1000 mW
(output format: 0, *.**E+**)

■ Suffix code

None

■ Initial setting

None

■ Example

SWPWR?␣UP2,WATT

SYMTIME Symbol Timing

■ Function Sets a symbol timing on the parameter setting screen.

Header	Program command	Query	Response
SYMTIME	SYMTIME␣a	SYMTIME?	a

■ Value of a −0.20 to 0.20 symbol (0.01 symbol steps)
■ Suffix code None
■ Initial setting Ø.ØØ
■ Example SYMTIME␣Ø.Ø2

SYS System

■ Function Sets a communication system.

Header	Program command	Query	Response
SYS	SYS␣a	SYS?	a

■ Value of a PDC (JDC), PHS (JDCT), NADC, PWRMTR
■ Suffix code None
■ Example SYS␣PHS

TEMPLVL

TEMPLVL Template-Level Modify

■ Function Creates a template on the template creation screen.

Header	Program command	Query	Response
TEMPLVL	TEMPLVL␣a,b	TEMPLVL?␣a	b

■ Value of a
1: Limit 1
2: Limit 2
3: Limit 3
4: Limit 4
5: Limit 5

■ Value of b −110.0 to 10.0 dB (0.1 steps)

■ Suffix code None

■ Initial setting (Units: dB)

	PDC	PHS	NADC
1: Limit 1	−70	−56	−60
2: Limit 2	−60	−56	−60
3: Limit 3	4	4	3
4: Limit 4	−60	−56	−60
5: Limit 5	−14	−14	−20

■ Example TEMPLVL?␣3

TERM Terminal

■ Function Sets the INPUT terminal on the parameter setting screen.

Header	Program command	Query	Response
TERM	TERM␣a	TERM?	a

■ Value of a
RF: RF
IQAC: I, Q - AC (option 03)
IQDC: I, Q - DC (option 03)

■ Suffix code None

■ Initial setting RF

■ Example TERM␣IQAC

TIMING? Timing

■ Function Outputs the measurement result Timing on the power measurement screen.

Header	Program command	Query	Response
TIMING	———	TIMING?	a,b

■ Value of a Measurement result classification flag

■ Value of b Outputs the measurement result in bit units.

■ Example TIMING?

TXPWR?

TXPWR? TX Power

■ Function Outputs the TX power of a measurement result on the power measurement screen.

Header	Program command	Query	Response
TXPWR	———	TXPWR?	a,b
	———	TXPWR?␣DBM	a,c
	———	TXPWR?␣WATT	a,d

■ Value of a Measurement result classification flag

■ Value of b Depends on displayed units

■ Value of c (dBm value) −70.46 to 40.42
(output format: 0, *****)

■ Value of d (Watt value) 0.1 nW to 10 W
(output format: 0, *.**E+**)

■ Suffix code None

■ Example TXPWR?

TXTIME

TXTIME Transmit Timing

■ Function Sets the Transmit Timing on the parameter setting screen.

Header	Program command	Query	Response
TXTIME	TXTIME␣a	TXTIME?	a

■ Value of a OFF, ON

■ Example TXTIME␣ON

UCAL User Cal. Factor

■ Function Sets the User Cal.Factor of the power meter screen.

Header	Program command	Query	Response
UCAL	UCAL␣a	UCAL?	a

■ Value of a −30.00 to 30.00 dB (0.01 steps)

■ Suffix code dB

■ Initial setting Ø

■ Example UCAL␣3.Ø

UNIT

UNIT Unit

■ Function

Sets the units of the power measurement, adjacent channel leakage power measurement, or spurious measurement screen.

Header	Program command	Query	Response
UNIT	UNIT␣a	UNIT? (Use the current screen.)	a
	———	UNIT?␣RFPWR (Use this query when reading the units of the power measurement screen from a screen other than the power measurement screen.)	a
	———	UNIT?␣ADJ (Use this query when reading the units of the adjacent channel leakage power measurement screen from a screen other than the adjacent channel leakage power measurement screen.)	a
	———	UNIT?␣SPURIOUS (Use this query when reading the units of the spurious measurement screen from a screen other than the spurious measurement screen.)	a

■ Value of a

DBM: dBm
Use this value on the power measurement, adjacent channel leakage power measurement, or spurious measurement screen.

WATT: nW/μW/mW/W
Use this value on the power measurement screen.

MW: mW
Use this value on the adjacent channel leakage power measurement or spurious measurement screen.

UW: μW
Use this value on the adjacent channel leakage power measurement or spurious measurement screen.

NW: nW
Use this value on the adjacent channel leakage power measurement or spurious measurement screen.

DB: dB
Use this value on the adjacent channel leakage power measurement or spurious measurement screen.

■ Suffix code None

■ Initial setting DBM

■ Example UNIT␣WATT

UNT Unit for Log Scale

■ Function Sets the display unit systems in LOG scale mode.

Header	Program command	Query	Response
UNT	UNT␣a a=0 ————	UNT? UNT?	UNT␣a a=0 UNT␣b

■ Value of a
Ø: dBm
Used for the power measurement, adjacent channel leakage power measurement or suprious measurement screen.

■ Value of b
WATT: nW/μW/mW/W
Used for the power measurement screen.
MW: mW
Used for the adjacent channel leakage power measurement or suprious measurement screen.
UW: μW
Used for the adjacent channel leakage power measurement or suprious measurement screen.
NW: nW
Used for the adjacent channel leakage power measurement or suprious measurement screen.
DB: dB
Used for the adjacent channel leakage power measurement or suprious measurement screen.

■ Suffix code None

■ Initial setting Ø: dBm

■ Example UNT␣Ø

AVG

AVG Average

Function

Sets averaging processing of the power and pccupied bandwidth and adjacent channel leakage power measurement screens.

Header	Program command	Query	Response
VAVG	VAVG␣sw VAVG␣a	VAVG?	a a=2 to 99

Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

Value of a
2 to 99 (1step): Averaging rate to process

Suffix code
None

Initial setting
4: 4 times

Example
VAVG␣ON
VAVG␣16

VECTERR?

ECTERR? RMS Vector Error

Function

Outputs the RMS vector error of a measurement result on the modulation analysis screen.

Header	Program command	Query	Response
VECTERR	———	VECTERR?	a,b

Value of a
Measurement result classification flag

Value of b
−327.68 % to 327.67 % (rms) (0.01 % steps)

Suffix code
None

Example
VECTERR?

WINDOW Winwow

■ Function Sets a window on the power measurement screen.

Header	Program command	Query	Response
WINDOW	WINDOW␣a	WINDOW?	a

■ Value of a

SLOT: Slot
FRAME: Frame
LEAD: Leading
RISE: Leading ——— Program commands only
TRAIL: Trailing
FALL: Trailing ——— Program commands only

■ Suffix code None

■ Initial setting SLOT

■ Example WINDOW␣FRAME

ZAJ Zero Adjust

■ Function Sets the power meter screen to zero (same function as ZEROSET).

Header	Program command	Query	Response
ZAJ	ZAJ	———	———

■ Suffix code None

■ Initial setting None

■ Example ZAJ

ZEROSET

ZEROSET Zero Set

■ Function Executes the zero set on the power meter screen.

Header	Program command	Query	Response
ZEROSET	ZEROSET	———	———

■ Suffix code None

■ Initial setting None

■ Example ZEROSET

(Blank)

6.4 Spectrum mode commands

AAT RF Attenuator

■ Function Switches the RF attenuator setting mode to AUTO or MANUAL.

Header	Program command	Query	Response
AAT	AAT␣a a=0, 1	AAT?	AAT␣a a=0, 1

■ Value of a
Ø: MANUAL
1: AUTO

■ Suffix code None

■ Initial setting 1: AUTO

■ Example AAT␣1

AMD Trace A Storage Mode

■ Function Selects the mode for processing trace A waveform.

Header	Program command	Query	Response
AMD	AMD␣a a=0 to 5	AMD?	AMD␣a a=0 to 5

■ Value of a
Ø: NORMAL
1: MAX HOLD
2: AVERAGE
3: MIN HOLD
4: CUMULATIVE
5: OVER WRITE

■ Suffix code None

■ Initial setting Ø: NORMAL

■ Example AMD␣Ø

ARB

ARB Resolution Band Width

■ Function Switches the mode for setting resolution bandwidth to AUTO or MANUAL.

Header	Program command	Query	Response
ARB	ARB␣a a=0, 1	ARB?	ARB␣a a=0, 1

■ Value of a Ø: MANUAL
1: AUTO

■ Suffix code None

■ Initial setting 1: AUTO

■ Example ARB␣Ø
ARB␣1

AST

AST Sweep Time

■ Function Switches the mode for setting frequency sweep time to AUTO or MANUAL.

Header	Program command	Query	Response
AST	AST␣a a=0, 1	AST?	AST␣a a=0, 1

■ Value of a Ø: MANUAL
1: AUTO

■ Suffix code None

■ Initial setting 1: AUTO

■ Example AST␣Ø
AST␣1

ASWT Auto Sweep Time

■ Function Sets the auto sweep time.

Header	Program command	Query	Response
ASWT	ASWT␣sw sw=FAST, SLOW	ASWT?	SW sw=FAST, SLOW

■ Value of sw
FAST: FAST
SLOW: SLOW

■ Suffix code None

■ Initial setting SLOW (provided the address already allocated is not initialized)

■ Example
ASWT␣FAST
ASWT␣SLOW

AT RF Attenuator

■ Function Sets the RF attenuator.

Header	Program command	Query	Response
AT	AT␣a	AT?	a

■ Value of a
AUTO: AUTO
UP: UP
DN: DOWN
Ø to 75: 20 to 75 dB (5 dB step)

■ Suffix code
None: dB
DB: dB

■ Initial setting Calculated value when AUTO is selected for ATT

■ Example
AT␣1Ø
AT␣55

ATT

ATT RF Attenuator

■ Function Sets the RF attenuator.

Header	Program command	Query	Response
ATT	ATT␣a a=0 to 11	ATT?	ATT␣a a=0 to 11

■ Value of a

LOW/HIGH		LOW/HIGH	
Ø:	0/20 dB	6:	5/25 dB
1:	10/30 dB	7:	15/35 dB
2:	20/40 dB	8:	25/45 dB
3:	30/50 dB	9:	35/55 dB
4:	40/60 dB	1Ø:	45/65 dB
5:	50/70 dB	11:	55/75 dB

■ Suffix code None

■ Initial setting Calculated value when AUTO is selected for ATT

■ Example ATT␣1

ATUN

ATUN Auto Tune

■ Function Executes automatic tuning.

Header	Program command	Query	Response
ATUN	ATUN	———	———

■ Example ATUN

■ Notes Automatic tuning terminates when the parameters for the next sweep were set. After executing the ATUN command, wait for the sweep to terminate before executing the next command.

AUNITS Unit for Log Scale

■ Function Sets one of the display unit systems when the LOG scale is selected.

Header	Program command	Query	Response
AUNITS	AUNITS␣a a=DBM, DBUV, DBMV, DBUVE, V	AUNITS?	a a=DBM, DBUV, DBMV, DBUVE, V

■ Value of a
DBM: dBm
DBUV: dBμV
DBMV: dBmV
DBUVE: dBmV (emf)
V: V

■ Suffix code None

■ Initial setting DBM: dBm (provided the address already allocated is not initialized)

AUTO Coupled Function All Auto

■ Function Executes all coupled functions (RBW, VBW, SWT, ATT) setting in AUTO mode.

Header	Program command	Query	Response
AUTO	AUTO	———	———

■ Example
```
AUTO
```

AVB

AVB Video Band Width

■ Function Switches the mode for setting the video bandwidth to AUTO or MANUAL.

Header	Program command	Query	Response
AVB	AVB␣a a=0, 1, 2	AVB?	AVB␣ a a=0, 1, 2

■ Value of a
Ø: MANUAL
1: AUTO
2: OFF

■ Suffix code None

■ Initial setting 1: AUTO

■ Example
AVB␣Ø
AVB␣1

AVR

AVR Number of Trace Average

■ Function Sets the averaging rate (number of sweep repetitions) to average the trace display.

Header	Program command	Query	Response
AVR	AVR␣a a=0 to 4	AVR?	AVR␣a a=0 to 4

■ Value of a
Ø: 4 times
1: 8 times
2: 16 times
3: 32 times
4: 128 times

■ Suffix code None

■ Initial setting 1: 8 times

■ Example
AVR␣Ø
AVR␣3

AWR Trace A Write Switch

■ Function Controls writing the waveform data to trace A.

Header	Program command	Query	Response
AWR	AWR␣a a=ON, 1, OFF, 0	AWR?	AWR␣a a=ON, OFF

■ Value of a
ON: TRACE A WRITE ON (Same function as CLRW␣TRA)
1: TRACE A WRITE ON (Same function as CLRW␣TRA)
OFF: TRACE A WRITE OFF (Same function as VIEW␣TRA)
Ø: TRACE A WRITE OFF (Same function as VIEW␣TRA)

■ Suffix code None

■ Initial setting 1: TRACE A WRITE ON

■ Example AWR␣Ø

A1 Trace A Write ON

■ Function Clears trace A (FREQ) waveform data to set the write mode to ON. (same function as AWR␣1/CLRW␣TRA)

Header	Program command	Query	Response
A1	A1	———	———

■ Example A1

A2

A2 Trace A Max Hold

■ Function

Allows trace A (FREQ) waveform to be processed in MAX HOLD mode (same function as AMD␣1).

Header	Program command	Query	Response
A2	A2	———	———

■ Example

A2

BNDC

BNDC Band Select

■ Function

Selects one of the bands in the frequency range of 0 to 8.5 GHz.

Header	Program command	Query	Response
BNDC	BNDC␣a a=AUTO, 0, 1^-, 1^+	BNDC?	BNDC␣a a=AUTO, 0, 1^-, 1^+

■ Value of a

AUTO:	BAND AUTO	=0 Hz to 8.5 GHz
Ø:	BAND 0	=0 Hz to 2 GHz
1−:	BAND 1^-	=1.7 GHz to 7.5 GHz
1+:	BAND 1^+	=6.5 GHz to 8.5 GHz

■ Suffix code

None

■ Initial setting

AUTO: BAND AUTO =0 Hz to 8.5 GHz

■ Example

BNDC␣AUTO
BNDC␣1+

BSAUTO BW/SWT Auto

■ Function Allows RBW, VBW, and sweep time to be set in AUTO mode.

Header	Program command	Query	Response
BSAUTO	BSAUTO	———	———

■ Example BSAUTO

CA RF Attenuator Auto

■ Function Sets the attenuator to AUTO mode (same function as AAT␣1, AT␣AUTO).

Header	Program command	Query	Response
CA	CA	———	———

■ Example CA

CAL

CAL Calibration

■ Function Selects the way of calibrating this instrument using internal CAL signal.

Header	Program command	Query	Response
CAL	CAL␣a a=0 to 2	———	———

■ Value of a
Ø: All
1: Frequency
2: Level

■ Suffix code None

■ Example
```
CAL␣Ø
```

CF

CF Center Frequency

■ Function Sets the center frequency (same function as CNF).

Header	Program command	Query	Response
CF	CF␣f CF␣a	CF?	f f= −100000000 to 0 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f −100 MHz to 8.5 GHz

■ Value of a
UP: CENTER FREQ STEP UP (Same function as FUP)
DN: CENTER FREQ STEP DOWN (Same function as FDN)

■ Suffix code
f: None: Hz (10^0)
HZ: Hz (10^0)
KHZ,KZ: kHz (10^3)
MHZ,MZ: MHz (10^6)
GHZ,GZ: GHz (10^9)

a: None

■ Initial setting Value of f = 4.25 GHz

■ Example
```
CF␣1235456
CF␣5ØMHz
CF␣UP
```

CLRW Clear & Write

■ Function Clears the trace waveform data to set the write mode to ON.

Header	Program command	Query	Response
CLRW	CLRW␣tr	———	———

■ Value of tr
TRA: Trace A (same function as AWR␣1)
TRTIME: Trace TIME (same function as TMWR␣1)

■ Example CLRW␣TRA

CMK? Current Marker Position

■ Function Reads the current marker position.

Header	Program command	Query	Response
CMK?	———	CMK?	CMK␣a a=0 to 500

■ Value of a 0 to 500

■ Example CMK?

CNF

CNF Center Frequency

■ Function Sets the center frequency (same function as CF).

Header	Program command	Query	Response
CNF	CNF␣f	CNF?	CNF␣f f= −100000000 to 0 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f −100 MHz to 8.5 GHz

■ Suffix code
None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Initial setting Value of f = 4.25 GHz

■ Example
```
CNF␣123456
CNF␣5ØMHZ
CNF?
```

COUPLE

COUPLE Coupling Mode

■ Function Switches the coupling to AC or DC to monitor FM waveform.

Header	Program command	Query	Response
COUPLE	COUPLE␣sw	COUPLE?	sw sw = AC, DC

■ Value of sw
AC: AC COUPLING
DC: DC COUPLING

■ Suffix code None

■ Initial setting AC: AC COUPLING

■ Example
```
COUPLE␣AC
COUPLE␣DC
```

CR Resolution Band Width Auto

■ Function

Sets the resolution bandwidth selection to the AUTO mode (same function as ARB_1, RB_AUTO).

Header	Program command	Query	Response
CR	CR	————	————

■ Example

```
CR
```


CT Sweep Time Auto

■ Function

Sets the frequency sweep time to AUTO mode (same function as AST_1, ST_AUTO).

Header	Program command	Query	Query
CT	CT	————	————

■ Example

```
CT
```

CV

CV Video Band Width Auto

■ Function Sets the video bandwidth to AUTO mode (same function as AVB␣1, VB␣AUTO).

Header	Program command	Query	Response
CV	CV	———	———

■ Example CV

DET

DET Detection Mode

■ Function Selects the detection mode of the waveform data being displayed.

Header	Program command	Query	Response
DET	DET␣d d=0 to 2 POS, SMP, NEG	DET?	d d=POS, SMP, NEG

■ Value of d
Ø: POSITIVE PEAK
1: SAMPLE
2: NEGATIVE PEAK
POS: POSITIVE PEAK
SMP: SAMPLE
NEG: NEGATIVE PEAK

■ Suffix code None

■ Initial setting Ø: POSITIVE PEAK

■ Example
DET␣Ø
DET␣SMP

DETM Detection Mode

■ Function Selects the detection mode of the trace specified to A or B.

Header	Program command	Query	Response
DETM	DETM␣tr,sw	DETM?␣tr	sw sw=POS, SMP, NEG

■ Value of tr TRA: Trace A

■ Value of sw POS: POSITIVE PEAK
SMP: SAMPLE
NEG: NEGATIVE PEAK

■ Suffix code None

■ Initial setting POS: POSITIVE PEAK

■ Example DETM␣TRA,POS

DFMT Display Format

■ Function Specifies the format used in the display mode / display.

Header	Program command	Query	Response
DFMT	DFMT␣sw	DFMT?	SW sw=A, TIME

■ Value of sw A: Trace A
TIME: Trace TIME

■ Suffix code None

■ Initial setting A: Trace A

■ Example DFMT␣TIME

DPOINT

DPOINT Data Point

■ Function Sets the data point

Header	Program command	Query	Response
DPOINT	DPOINT␣SW sw=NRM, DOUBLE	DPOINT?	SW sw=NRM, DOUBLE

■ Value of sw NRM: NORMAL
DOUBLE: DOUBLE

■ Suffix code None

■ Initial setting NRM: NORMAL (provided the address already allocated is not initialized)

■ Example DPOINT␣NRM

EXTTYPE

EXTTYPE Ext Trigger Input Type

■ Function Chooses the level input from the external trigger when EXT is selected for trigger source.

Header	Header	Query	Response
EXTTYPE	EXTTYPE␣SW	EXTTYPE?	SW sw=10 V, TTL

■ Value of sw 10V: INPUT 1 (±10V)
TTL: INPUT 2 (TTL)

■ Suffix code None

■ Initial setting 10V: INPUT 1 (±10V)

■ Example EXTTYPE␣10V
EXTTYPE␣TTL

E1 Peak Search

■ Function Executes the function for peak search (same function as MKS_0, MKMP).

Header	Program command	Query	Response
E1	E1	———	———

■ Example E1

E2 Marker to CF

■ Function Sets the marker frequency to the center frequency (same function as MKR_3, MKCF).

Header	Program command	Query	Response
E2	E2	———	———

■ Example E2

E3

E3 Marker to CF Step Size

■ Function

Sets the marker frequency to the frequency step size (same function as MKR_5, MKSS).

Header	Program command	Query	Response
E3	E3	———	———

■ Example

```
E3
```

E4

E4 Marker to REF

■ Function

Sets the marker level to the reference level (same function as MKR_4, MKRL).

Header	Program command	Query	Response
E4	E4	———	———

■ Example

```
E4
```

FA Start Frequency

■ Function Sets the start frequency (same function as STF).

Header	Program command	Query	Response
FA	FA␣f	FA?	f f= −100000000 to 0 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f −100 MHz to 8.5 GHz

■ Suffix code
None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Initial setting Value of f = 0 Hz

■ Example FA␣1GZ

FB Stop Frequency

■ Function Sets the stop frequency (same function as SOF).

Header	Program command	Query	Response
FB	FB␣f	FB?	f f= −100000000 to 0 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f −100 MHz to 8.5 GHz

■ Suffix code
None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Initial setting Value of f = 8.5 GHz

■ Example FB␣5GHZ

FDN

FDN Center Frequency Step Down

■ Function Decreases the center frequency by the frequency step size, if it has been set (same function as CF␣DN).

Header	Program command	Query	Response
FDN	FDN	———	———

■ Example FDN

FMRNG

FMRNG FM Range

■ Function Sets the bandwidth for demodulating FM when trace TIME is selected for FM monitoring

Header	Program command	Query	Response
FMRNG	FMRNG␣f	FMRNG?	f f=2000 to 200000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f
2 kHz/div
20 kHz/div
200 kHz/div

■ Suffix code
None: Hz/div
HZ: Hz/div
KHZ, KZ: kHz/div
MHZ, MZ: MHz/div
GHZ, GZ: GHz/div

■ Initial setting 200 kHz/div

■ Example FMRNG␣2ØKHZ

FRQ Frequency Mode

■ Function Selects the mode for setting the frequency band.

Header	Program command	Query	Response
FRQ	FRQ␣a a=0 to 2	FRQ?	FRQ␣a a=0 to 2

■ Value of a
Ø: CENTER-SPAN
1: START-SPAN
2: START-STOP

■ Suffix code None

■ Initial setting 2: START-STOP

■ Example
FRQ␣Ø
FRQ␣1

FS Full Span

■ Function ets the frequency span to the full span that is the maximum value settable in the frequency band being set.

Header	Program command	Query	Response
FS	FS	———	———

■ Example FS

FSS

FSS Frequency Step Size

■ Function — Sets the frequency step size for stepping up/down the frequency (same function as SS).

Header	Program command	Query	Response
FSS	FSS␣f	FSS?	FSS␣f f=1 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f — 1 Hz to 8.5 GHz

■ Suffix code

None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Initial setting — 1 GHz

■ Example

```
FSS␣1GHZ
FSS␣1000
```

FUP

FUP Frequency Step Up

■ Function — Increases the center frequency by the frequency step size, if it has been set (same function as FREQ␣UP).

Header	Program command	Query	Response
FUP	FUP	———	———

■ Example

```
FUP
```

GATE Gate Sweep ON/OFF

■ Function Allows the gate function to be set to ON or OFF

Header	Program command	Query	Response
GATE	GATE␣sw sw=ON, 1, OFF, 0	GATE?	sw sw=ON, OFF

■ Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code None

■ Initial setting OFF: OFF

■ Example GATE␣ON

GD Gate Delay

■ Function Sets the delay time of gate.

Header	Program command	Query	Response
GD	GD␣t	GD?	t t=0 to 65500 Transfers the data without suffix code as if represented in units of μsec.

■ Value of t 0 to 65.5 msec

■ Suffix code
None: msec
US: μsec
MS: msec
S: sec

■ Initial setting Value of t = 0 sec

■ Example GD␣2ØMS

GE

GE Gate End

■ Function Allows the interval of gate to be ended internally or externally.

Header	Program command	Query	Response
GE	GE␣SW sw=INT, EXT	GE?	SW sw=INT, EXT

■ Value of sw
INT: INTERNAL (inside)
EXT: EXTERNAL (outside)

■ Suffix code None

■ Initial setting INT: INTERNAL (inside)

■ Example GE␣INT

GL

GL Gate Length

■ Function Sets the length of gate.

Header	Program command	Query	Response
GL	GL␣t	GL?	t t=20 to 65500 Transfers the data without suffix code as if represented in units of μsec

■ Value of t 20 μsec to 65.5 msec

■ Suffix code
None: msec
US: μsec
MS: msec
S: sec

■ Initial setting Value of t = 1 msec

■ Example GL␣2ØMS

HN Band Select

■ Function Selects one of the bands in the frequency range from 0 to 8.5 GHz.

Header	Program command	Query	Response
HN	HN␣a a=0 to 2	HN?	a a=0 to 2 ***

■ Value of a
Ø: BAND0
1: BAND1⁻
2: BAND1⁺

■ Suffix code None

■ Initial setting (BAND␣AUTO)

■ Example HN␣Ø

Note: The response when the band is selected for BAND AUTO becomes " *** ".

HNLOCK Band Select

■ Function Selects one of the bands in the frequency range from 0 to 8.5 GHz.

Header	Program command	Query	Response
HNLOCK	HNLOCK␣a a=0 to 2, OFF	HNLOCK?	HNLOCK␣b b=ON, OFF

■ Value of a
Ø: BAND0 (Same function as BNDC␣Ø)
1: BAND1⁻ (Same function as BNDC␣1-)
2: BAND1⁺ (Same function as BNDC␣1+)
OFF: BAND AUTO (Same function as BNDC␣AUTO)

■ Value of b
ON: BAND 0, 1⁻. 1⁺
OFF: BAND AUTO

■ Suffix code None

■ Initial setting OFF: BAND AUTO

■ Example HNLOCK␣2

HNUNLK

HNUNLK Band Select

■ Function

Allows the bands to be selected in the AUTO mode (Same function as BNDC_AUTO, HNLOCK_OFF).

Header	Program command	Query	Response
HNUNLK	HNUNLK	———	———

■ Example

```
HNUNLK
```

KSA

KSA Unit for Log Scale

■ Function

Sets the unit system of LOG scale to dBm (same function as UNT_0).

Header	Program command	Query	Response
KSA	KSA	———	———

■ Example

```
KSA
```

KSB Unit for Log Scale

■ Function Sets the unit system of LOG scale to dBmV (same function as UNT_2).

Header	Program command	Query	Response
KSB	KSB	———	———

■ Example KSB

KSC Unit for Log Scale

■ Function Sets the unit system of LOG scale to dBμV (same function as UNT_1).

Header	Program command	Query	Response
KSC	KSC	———	———

■ Example KSC

KSD

KSD Unit for Log Scale

■ Function Sets the unit system of LOG scale to V (same function as UNT_3).

Header	Program command	Query	Response
KSD	KSD	———	———

■ Example KSD

KSG

KSG Average ON

■ Function Allows the averaging to be used when set to ON.

Header	Program command	Query	Response
KSG	KSG	———	———

■ Example KSG

KSH Average OFF

■ Function

Turns off the averaging operation to set the mode for processing waveform to NORMAL.

Header	Program command	Query	Response
KSH	KSH	———	———

■ Example

```
KSH
```


KSO Delta Marker to Span

■ Function

Sets the delta marker frequency to frequency span (same function as MKR→6, MKSP).

Header	Program command	Query	Response
KSO	KSO	———	———

■ Example

```
KSO
```

LG

LG Scale

■ Function Sets the magnification of Y axis and scale.

Header	Program command	Query	Response
LG	LG␣ℓ LG␣a	LG?	ℓ ℓ=0, 1, 2, 5, 10

■ Value of ℓ
- Ø: Sets the scaling function to linear mode.
- 1: 1 dB/div (Sets the scaling function to logarithmic mode)
- 2: 2 dB/div (Sets the scaling function to logarithmic mode)
- 5: 5 dB/div (Sets the scaling function to logarithmic mode)
- 1Ø: 10 dB/div (Sets the scaling function to logarithmic mode)

■ Value of a
- UP: SCALE UP
- DN: SCALE DOWN

■ Suffix code
- None: dB/div
- DB, DBM, DM: dB/div

■ Initial setting 1Ø: 10 dB/div

■ Example
```
LG␣UP
LG␣5DB
```

LN

LN Linear Scale

■ Function Sets the magnification of Y axis and scale.

Header	Program command	Query	Response
LN	LN	———	———

■ Example
```
LN
```

LSS Reference Level Step Size (Manual)

■ Function — Sets the step size (manual values) of reference level increasing or decreasing in the specified step level.

Header	Program command	Query	Response
LSS	LSS␣ℓ	LSS?	LSS␣ℓ ℓ=0.1 to 100.0 Transfers the data without suffix code as if represented in units of dB

■ Value of ℓ — 0.1 to 100.0 dB (0.1dB step)

■ Suffix code — None: dB
DB, DBM, DM: dB

■ Initial settin — Value of ℓ = 1 dB

■ Example
LSS␣6
LSS␣1Ø

LSSA Reference Level Step Size (Auto)

■ Function — Sets the step size (auto values) of reference level increasing or decreasing in the specified step level during LOG SCALE.

Header	Program command	Query	Response
LSSA	LSSA␣a	LSSA?	LSSA␣a a=1, 2, 5, 10

■ Value of a
1: 1 div
2: 2 div
5: 5 div
1Ø: 10 div

■ Suffix code — None

■ Initial setting — 1: 1 div

■ Example — LSSA␣1Ø

MKA?

MKA? Marker Level Read

■ Function Reads out the level data at the marker point. At the delta marker point, the level differences are read out (same function as MKL?).

Header	Program command	Query	Response
MKA?	———	MKA?	ℓ v f

■ Value of ℓ No unit, Level data with 1 dB unit (when display unit system for marker level is dB), Resolution 0.01 dB

■ Value of v No unit, Level data with 1 nV unit (when display unit system for marker level is V), Resolution 0.1 nV
No unit, Level data with 1 V unit (for EXT TRIG MONITOR), Resolution 0.001 V

■ Value of f No unit, Frequency data with 1 Hz unit (for FM MONITOR), Resolution 1 Hz

■ Example MKA?

MKACT

MKACT Marker Active

■ Function Selects the active marker among the multimarkers.

Header	Program command	Query	Response
MKACT	MKACT␣a a=1 to 10	MKACT?	a a=1 to 10

■ Value of a 1 to 10 (multimarker No.)

■ Suffix code None

■ Initial setting 1: 1

■ Example MKACT␣1

MKCF Marker to CF

■ Function

Sets the marker frequency to the center frequency (same function as MKR ␣3, E2).

Header	Program command	Query	Response
MKCF	MKCF	———	———

■ Example

```
MKCF
```


MKD Delta Marker Mode

■ Function

Sets the marker mode to delta marker mode.

Header	Program command	Query	Response
MKD	MKD	———	———

■ Example

```
MKD
```

MKF?

MKF? Marker Frequency Read

■ Function — Reads out the frequency or time data at the marker point. At the delta marker mode, the frequency or time differences are read out.

Header	Program command	Query	Response
MKF?	———	MKF?	f t

■ Value of f — No unit, frequency data with 1 Hz unit, Resolution 0.1 Hz

■ Value of t — No unit, time data with 1 μs unit, Resolution 0.1 μsec

■ Example — MKF?

MKL?

MKL? Marker Level Read

■ Function — Reads out the level data at the marker point. At the delta marker mode, the level differences are read out.

Header	Program command	Query	Response
MKL?	———	MKL?	ℓ v f

■ Value of ℓ — No unit, Level data with 1 dB unit (when display unit system for marker level is dB), Resolution 0.01 dB

■ Value of v — No unit, Level data with 1 nV unit (when display unit system for marker level is V), Resolution 0.1 nV
No unit, Level data with 1 V unit (for EXT TRIG MONITOR), Resolution 0.001 V

■ Value of f — No unit, Frequency data with 1 Hz unit (for FM MONITOR), Resolution 1 Hz

■ Example — MKL?

MKLIST Multi Marker List

■ Function Turns ON or OFF the multimarker list.

Header	Program command	Query	Response
MKLIST	MKLIST␣SW sw=ON, 1, OFF, 0	MKLIST?	SW sw=ON,OFF

■ Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code None

■ Initial setting OFF: OFF

■ Example
```
MKLIST␣ON
```


MKMCL Clear Multi Marker

■ Function Clears all the registered multimarkers.

Header	Program command	Query	Response
MKMCL	MKMCL	———	———

■ Example
```
MKMCL
```

MKMHI

MKMHI Multi Marker

■ Function

Registers multimarkers on the peak point from the maximum level down to the tenth in descending order.

Header	Program command	Query	Response
MKMHI	MKMHI	———	———

■ Example

```
MKMHI
```

MKMHRM

MKMHRM Multi Marker

■ Function

Registers multimarkers on the harmonic frequency ranging from the reference active marker frequency up to the tenth.

Header	Program command	Query	Response
MKMHRM	MKMHRM	———	———

■ Example

```
MKMHRM
```

MKMIN Minimum Search

■ Function

Searches the spectrum being displayed for the minimum point and moves the marker to that point.

Header	Program command	Query	Response
MKMIN	MKMIN	———	———

■ Example

```
MKMIN
```


MKML? Multi Marker List Query (Level)

■ Function

Reads out the level data at multimarkers.

Header	Program command	Query	Response
MKML	———	MKML?␣a	ℓ v f

■ Value of a

1 to 10 (multimarker No.)

■ Value of ℓ

No unit, Level data with 1 dB unit (when display unit system for marker level is dB), Resolution 0.01 dB

■ Value of v

No unit, Level data with 1 nV unit (when display unit system for marker level is V), Resolution 0.1 nV
No unit, Level data with 1 V unit (for EXT TRIG MONITOR) Resolution 0.001 V

■ Value of f

No unit, Frequency data with 1 Hz unit (for FM MONITOR) Resolution 1 Hz

■ Suffix code

None

MKMP

MKMP Marker Position

■ Function Specifies the frequency of the designated multimarker number.

Header	Program command	Query	Response
MKMP	MKMP␣a,f	MKMP?␣a a=1 to 10	f f=−100000000 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of a 1 to 10 (Multimarker No.)

■ Value of f −100 MHz to 8.5 GHz

■ Suffix code
None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Example MKMP␣5,2400MHZ

MKMULTI

MKMULTI Multi Marker

■ Function Turns ON or OFF the multimarker.

Header	Program command	Query	Response
MKMULTI	MKMULTI␣sw sw=ON, 1, OFF, 0	MKMULTI?	SW sw=ON, OFF

■ Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code None

■ Initial setting OFF: OFF

■ Example MKMULTI␣ON

MKN Marker Position

■ Function — Specifies the zone marker center position on the X axis in the frequency or time unit.

Header	Program command	Query	Response
MKN	MKN␣f MKN␣t MKN␣a	MKN?	f,t f=−100000000 to 0 to 8500000000 Transfers the data without suffix code as if represented in units of Hz t=−1000000000 to1 000000000 Transfers the data without suffix code as if represented in units of μsec

■ Value of f — −100 MHz to 8.5 GHz
(0 to 8.5 GHz (specified when the valid trace is A, B, or BG)

■ Value of t — −1000 sec to 1000 sec (specified when the valid trace is TIME)

■ Value of a
UP: UP
DN: DOWN

■ Suffix code

f:		t:	
None:	Hz (10^0)	None:	msec
HZ:	Hz (10^0)	US:	μsec
KHZ, KZ:	kHz (10^3)	MS:	msec
MHZ, MZ:	MHz (10^6)	S:	sec
GHZ, GZ:	GHz (10^9)		

■ Example
MKN␣100MHZ
MKN␣UP

MKOFF Marker Mode

■ Function — Turns off the marker mode.

Header	Program command	Query	Response
MKOFF	MKOFF␣a	———	———

■ Value of a
ALL: Marker off
None: Marker off

■ Suffix code — None

■ Example
MKOFF␣ALL
MKOFF

MKP

MKP Marker Position

■ Function

Specifies the zone marker center position on the X axis in the point unit (same function as MKZ).

Header	Program command	Query	Response
MKP	MKP␣p	MKP?	p p=0 to 500

■ Value of p 0 to 500

■ Suffix code None

■ Initial setting Value of p = 250

■ Example
```
MKP␣25Ø
MKP␣5ØØ
```

MKPK

MKPK Peak Search

■ Function

Searches the spectrum being displayed for one of the special points and moves the marker to that point.

Header	Program command	Query	Response
MKPK	MKPK␣a	———	———

■ Value of a
```
None: SEARCH PEAK (MAX)
HI:   SEARCH PEAK (MAX)
NH:   SEARCH NEXT PEAK
NR:   SEARCH NEXT RIGHT PEAK
NL:   SEARCH NEXT LEFT PEAK
```

■ Suffix code None

■ Example
```
MKPK␣HI
MKPK␣NL
```

MKR Marker Mode

■ Function Switches the marker mode and executes the 'MKR to ' functions.

Header	Program command	Query	Response
MKR	MKR␣a a=0 to 7	MKR?	MKR␣a a=0 to 2

■ Value of a
Ø: NORMAL
1: DELTA
2: OFF
3: MKR to CF
4: MKR to REF
5: MKR to CFstep size
6: ␣MKR to SPAN
7: ZONE to SPAN

■ Suffix code None

■ Initial setting Ø: NORMAL

■ Example MKR␣Ø

MKRL Marker to REF

■ Function Sets the marker level to the reference level (same function as MKR␣4, E4)

Header	Program command	Query	Response
MKRL	MKRL	———	———

■ Example MKRL

MKS

MKS Peak Search

■ Function

Searches the spectrum being displayed for one of the special points and moves the marker to that point.

Header	Program command	Query	Response
MKS	MKS␣a a=0 to 2, 9 to 11	———	———

■ Value of a

Ø: SEARCH PEAK (MAX)
1: SEARCH NEXT PEAK
2: SEARCH DIP (MIN)
9: SEARCH NEXT RIGHT PEAK
1Ø: SEARCH NEXT LEFT PEAK
11: SEARCH NEXT DIP

■ Suffix code

None

■ Example

```
MKS␣Ø
MKS␣9
```

MKSLCT

MKSLCT Select Multi Marker

■ Function

Specifies one of the 1 to 10 multimarkers and sets the specified marker to ON or OFF.

Header	Program command	Query	Response
MKSLCT	MKSLCT␣a,sw a=1 to 10 sw=ON, 1, OFF, 0	MKSLCT?␣a a=1 to 10	sw sw=ON, OFF

■ Value of a

1 to 10 (multimarker No.)

■ Value of sw

ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code

None

■ Initial setting

OFF: OFF

■ Example

```
MKSLCT␣3,ON
```

MKSP Delta Marker to Span

■ Function

Sets the delta marker frequency to the span (same function as MKR_6, KSO).

Header	Program command	Query	Response
MKSP	MKSP	———	———

■ Example

```
MKSP
```


MKSS Marker to CF Step Size

■ Function

Sets the marker frequency as a frequency step size (same function as MKR_5, E3).

Header	Program command	Query	Response
MKSS	MKSS	———	———

■ Example

```
MKSS
```

MKTRACK

MKTRACK Tracking ON/OFF

■ Function Sets the signal tracking function to ON or OFF.

Header	Program command	Query	Response
MKTRACK	MKTRACK␣SW sw=ON, 1, OFF, 0	MKTRACK?	SW sw=ON, OFF

■ Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code None

■ Initial setting OFF: OFF

■ Example
```
MKTRACK␣ON
```

MKW

MKW Zone Marker Width

■ Function Specifies the zone marker width in the div unit.

Header	Program command	Query	Response
MKW	MKW␣a a=1 to 2, 5 to 7	MKW?	MKW␣a a=1 to 2, 5 to 7

■ Value of a
1: Spot
2: 10 div
5: 1 div
6: 2 div
7: 5 div

■ Suffix code None

■ Initial setting 5: 1 div

■ Example
```
MKW␣1
MKW␣5
```

MKZ Zone Marker Position

■ Function

Specifies the zone marker center position on the X axis in the point unit (same function as MKP).

Header	Program command	Query	Response
MKZ	MKZ␣p p=0 to 500	MKZ?	MKZ␣p p=0 to 500

■ Value of p 0 to 500

■ Suffix code None

■ Initial setting Value of p = 250

■ Example
```
MKZ␣25Ø
MKZ␣5ØØ
```


MKZF Zone Marker Position

■ Function

Specifies the zone marker center position on the X axis in frequency or time units.

Header	Program command	Query	Response
MKZF	MKZF␣f MKZF␣t	MKZF?	f t f=−100000000 to 0 to 8500000000 Transfers the data without suffix code as if represented in units of Hz t=−100000000 to 8500000000 Transfers the data without suffix code as if represented in units of μsec

■ Value of f −100 MHz to 8.5 GHz (specified when the valid trace is A, B, or BG)

■ Value of t −1000 sec to 1000 sec (specified when the valid trace is TIME)

■ Suffix code

f:			t:	
None:	Hz (10^0)		None:	msec
HZ:	Hz (10^0)		US:	μsec
KHZ, KZ:	kHz (10^3)		MS:	msec
MHZ, MZ:	MHz (10^6)		S:	sec
GHZ, GZ:	GHz (10^9)			

■ Example
```
MKZF␣1ØØMHZ
MKZF␣12ØØØØØØØØ
```

MON

MON Monitor Mode

■ Function Selects the function for monitoring the sound from the detector output.

Header	Program command	Query	Response
MON	MON␣m	MON?	m m=AM, FM, OFF

■ Value of m
AM: Amplitude Modulation
FM: Frequency Modulation
OFF: OFF

■ Suffix code None

■ Initial setting OFF: OFF

■ Example MON␣AM

MONVOL

MONVOL Monitor Volume

■ Function Adjusts the volume of sound monitor.

Header	Program command	Query	Response
MONVOL	MONVOL␣v v=0 to 20	MONVOL?	v v=0 to 20

■ Value of v 0 to 20 (1 step)

■ Suffix code None

■ Initial setting Value of v = 10

■ Example MONVOL␣1Ø

MTØ Tracking OFF

■ Function Sets the signal tracking function to OFF.

Header	Program command	Query	Response
MTØ	MTØ	———	———

■ Example MTØ

MT1 Tracking ON

■ Function Sets the signal tracking function to ON.

Header	Program command	Query	Response
MT1	MT1	———	———

■ Example MT1

MXMH

MXMH Max Hold

■ Function Sets the mode for processing the trace waveform to MAX HOLD.

Header	Program command	Query	Response
MXMH	MXMH␣tr	———	———

■ Value of tr TRA: Trace A (FREQ)

■ Suffix code None

■ Example MXMH␣TRA

MZW

MZW Zone Marker Width

■ Function Specifies the zone marker width on the X axis in the point unit.

Header	Program command	Query	Response
MZW	MZW␣w w = 1 to 501	MZW?	MZW␣w w = 1 to 501

■ Value of w 1 to 501 (odd number)

■ Suffix code None

■ Initial setting Value of w = 51

■ Example
MZW␣1
MZW␣51
MZW␣5Ø1

MZWF Zone Marker Width

■ Function Specifies the zone marker width on the X axis in the frequency.

Header	Program command	Query	Response
MZWF	MZWF␣f	MZWF?	f f=1 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f 1 Hz to 8.5 GHz

■ Suffix code
None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Initial setting frequency width equivalent to 1 div (850 MHz)

■ Example
MZWF␣100
MZWF␣1MHZ

M1 Marker Mode

■ Function Turns off the marker mode (same function as MKR␣2).

Header	Program command	Query	Response
M1	M1	———	———

■ Example M1

M2

M2 Marker Mode

■ Function Sets the marker mode to NORMAL mode (same function as MKR_0).

Header	Program command	Query	Response
M2	M2	———	———

■ Example M2

M3

M3 Marker Mode

■ Function Sets the marker mode to delta marker mode (same function as MKR_1).

Header	Program command	Query	Response
M3	M3	———	———

■ Example M3

PARAM Parameter

■ Function Displays the currently parameter list on the screen.

Header	Program command	Query	Response
PARAM	PARAM␣a	PARAM?	a a=1,2,OFF

■ Value of a
OFF: OFF
1: Parameter list 1
2: Parameter list 2

■ Suffix code None

■ Initial setting OFF: OFF

■ Example PARAM␣1

PCF Peak to Center Frequency

■ Function Searches the spectrum being displayed for the maximum point and sets the frequency at the point to the center frequency.

Header	Program command	Query	Response
PCF	PCF	———	———

■ Example PCF

PP

PP Presel Auto

■ Function Adjusts the bias of preselector automatically (same function as PRESEL␣AUTO).

Header	Program command	Query	Response
PP	PP	———	———

■ Example PP

PRESEL

PRESEL Presel Tune

■ Function Adjusts the bias of preselector.

Header	Program command	Query	Response
PRESEL	PRESEL␣a	PRESEL?	a a=−128 to 127

■ Value of a
AUTO: Automatic adjustment
−128 to 127: Setting values manually
PRESET: Sets 0

■ Suffix code None

■ Initial setting 0 (MANUAL) (provided the address already allocated is not initialized)

■ Example PRESEL␣AUTO

PRL Peak to Reference Level

■ Function

Searches the spectrum being displayed for the maximum point and sets its level to the reference level.

Header	Program command	Query	Response
PRL	PRL	———	———

■ Example

```
PRL
```


PSW Zone Sweep

■ Function

Sets the zone sweep to ON or OFF.

Header	Program command	Query	Response
PSW	PSW␣sw sw=ON, 1, OFF, 0	PSW?	PSW␣sw sw=ON, OFF

■ Value of sw

```
ON:  ON
1:   ON
OFF: OFF
Ø:   OFF
```

■ Suffix code

None

■ Initial setting

```
OFF: OFF
```

■ Example

```
PSW␣ON
```

RB

RB Resolution Band Width

■ Function Sets the resolution bandwidth (same function as RBW).

Header	Program command	Query	Response
RB	RB␣f RB␣a	RB?	f f=10 to 3000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f 10 Hz to 3 MHz (1-3 sequence)

■ Value of a
UP: RBW UP
DN: RBW DOWN
AUTO: RBW AUTO

■ Suffix code
f: None: Hz (10^0)
HZ: Hz (10^0)
KHZ,KZ: kHz (10^3)
MHZ,MZ: MHz (10^6)
GHZ,GZ: GHz (10^9)

a: None

■ Initial setting RBW = Calculated value when AUTO is selected for RBW.

■ Example RB␣3KHZ

RBW

RBW Resolution Band Width

■ Function Sets the resolution bandwidth.

Header	Program command	Query	Response
RBW	RBW␣a a=0 to 9, 13, 14	RBW?	RBW␣a a=0 to 9, 13, 14

■ Value of a
Ø: 30 Hz
1: 100 Hz
2: 300 Hz
3: 1 kHz
4: 3 kHz
5: 10 kHz
6: 30 kHz
7: 100 kHz
8: 300 kHz
9: 1 MHz
13: 10 Hz
14: 3 MHz

■ Suffix code None

■ Initial setting RBW = Calculated value when AUTO is selected for RBW

■ Example RBW␣5

RL Reference Level

■ Function Sets the reference level (same function as RLV).

Header	Program command	Query	Response
RL	RL␣ℓ RL␣a	RL?	ℓ ℓ: Available for the current scale unit, provided μV unit is always selected in LIN mode.

■ Value of ℓ Value equivalent to −100 dBm to +50 dBm (0.1 dB step)

■ Value of a
UP: LEVEL STEP UP
DN: LEVEL STEP DOWN

■ Suffix code

None:	Available for the current scale unit, provided μV unit is always selected in LIN mode
DB, DBM, DM:	dBm
DBMV:	dBmV
DBUV:	dBμV
DBUVE:	dBμV (emf)
V:	V
MV:	mV
UV:	μV
W:	W
MW:	mW
UW:	μW
NW:	nW
PW:	pW
FW:	fW

■ Initial setting Value of ℓ = 10 dBm

■ Example
```
RL␣−1ØØDBM
RL␣5V
RL␣−1Ø
RL␣UP
```

RLV

RLV Reference Level

■ Function Sets the reference level (same function as RL).

Header	Program command	Query	Response
RLV	RLV␣ℓ	RLV?	RLV␣ℓ ℓ: Transfers the data without suffix code as if represented in the current scale units (always μV unit in LIN mode).

■ Value of ℓ Value equivalent to −100 to +50 dBm
(0.1 dB step)

■ Suffix code

None:	Available for the current scale unit, provided μV unit is always selected in LIN mode
DB, DBM, DM:	dBm
DBMV:	dBmV
DBUV:	dBμV
DBUVE:	dBμV (emf)
V:	V
MV:	mV
UV:	μV

■ Initial setting Value of ℓ = 10 dBm

■ Example
```
RLV␣−7ØDBM
RLV␣5V
RLV␣−1Ø
```

RMK?

RMK? Reference Marker Position

■ Function Reads out the position of reference marker.

Header	Program command	Query	Response
RMK?	———	RMK?	RMK␣a

■ Value of a 0 to 500

■ Example
```
RMK?
```

SCL Log/Linear Scale

■ Function Sets the magnification of LOG/LIN scale (Y axis).

Header	Program command	Query	Response
SCL	SCL␣a a=0 to 7	SCL␣?	SCL␣a a=0 to 7

■ Value of a
Ø: 1 dB/div (LOG SCALE)
1: 2 dB/div (LOG SCALE)
2: 5 dB/div (LOG SCALE)
3: 10 dB/div (LOG SCALE)
4: 1 %/div (LIN SCALE)
5: 2 %/div (LIN SCALE)
6: 5 %/div (LIN SCALE)
7: 10 %/div (LIN SCALE)

■ Suffix code None

■ Initial setting 3: 10 dB/div (LOG SCALE)

■ Example
SCL␣Ø
SCL␣5

SOF Stop Frequency

■ Function Sets the stop frequency (same function as FB).

Header	Program command	Query	Response
SOF	SOF␣f	SOF?	SOF␣f f=−100000000 to 0 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f −100 MHz to 8.5 GHz

■ Suffix code
None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Initial setting Value of f = 8.5 GHz

■ Example
SOF␣123MHZ
SOF␣45.6KHZ

SP

SP Frequency Span

■ Function Sets the frequency span (same function as SPF).

Header	Program command	Query	Response
SP	SP␣f SP␣a	SP?	f f=0 to 8600000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f 0 Hz to 8.6 GHz

■ Value of a UP: FREQ SPAN STEP UP (Same function as SPU)
DN: FREQ SPAN STEP DOWN (Same function as SPD)

■ Suffix code None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Initial setting Value of f = 8.6 GHz

■ Example SP␣6GHZ

SPD

SPD Frequency Span Step Down

■ Function Decreases the frequency span in the 5-2-1 steps (same function as SP␣DN).

Header	Program command	Query	Response
SPD	SPD	———	———

■ Example SPD

SPF Frequency Span

■ Function Sets the frequency span (same function as SP).

Header	Program command	Query	Response
SPF	SPF␣f	SPF?	SPF␣f f=0 to 8600000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f 0 Hz to 8.6 GHz

■ Suffix code
None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Initial setting Value of f=8.6 GHz

■ Example
SPF␣1Ø1MHZ
SPF␣3.5GHZ

SPFUNC Time Trace Special Function

■ Function Sets the function for monitoring the trace time waveform (FM/TRIG MONITOR).

Header	Program command	Query	Response
SPFUNC	SPFUNC␣sw	SPFUNC?	sw sw=OFF, FM, EXT

■ Value of sw
OFF: OFF
FM: FM MONITOR
EXT: EXT TRIGGER MONITOR

■ Suffix code None

■ Initial setting OFF: OFF

■ Example SPFUNC␣FM

SPU

SPU Frequency Span Step Up

■ Function Increases the frequency span in the 1-2-5 steps (same function as SP␣UP).

Header	Program command	Query	Response
SPU	SPU	———	———

■ Example SPU

SS

SS Frequency Step Size

■ Function Sets the frequency step size for stepping up/down the frequency (same function as FSS).

Header	Program command	Query	Response
SS	SS␣f	SS?	f f=1 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f 1 Hz to 8.5 GHz

■ Suffix code
None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Example SS␣1MHZ

ST Sweep Time

■ Function Sets the frequency sweep time/time span.

Header	Program command	Query	Response
ST	ST␣t ST␣a	ST?	t t=50 to 1000000000 Transfers the data without suffix code as if represented in units of μsec

■ Value of t 50 μsec to 1000 sec (20 msec to 1000 sec for frequency axis)

■ Value of a
UP: SWT UP
DN: SWT DOWN
AUTO: SWT AUTO

■ Suffix code
t: None: msec
US: μsec
MS: msec
S: sec
a: None

■ Initial setting Calculated value when AUTO is selected for SWT

■ Example
ST␣AUTO
ST␣20MS

STF Start Frequency

■ Function Sets the start frequency (same function as FA).

Header	Program command	Query	Response
STF	STF␣f	STF?	STF␣f f=−100000000 to 0 to 8500000000 Transfers the data without suffix code as if represented in units of Hz

■ Value of f −100 MHz to 8.5 GHz

■ Suffix code
None: Hz (10^0)
HZ: Hz (10^0)
KHZ, KZ: kHz (10^3)
MHZ, MZ: MHz (10^6)
GHZ, GZ: GHz (10^9)

■ Initial setting Value of f = 0 Hz

■ Example
STF␣123MHZ
STF␣45.6KHZ

SWT

SWT Sweep Time

■ Function Sets the frequency sweep time/time span (same function as ST).

Header	Program command	Query	Response
SWT	SWT␣t	SWT?	SWT␣t t=50 to 1000000000 Transfers the data without suffix code as if represented in units of μsec

■ Value of t 50 μsec to 1000 sec (20 msec to 1000 sec for frequency axis)

■ Suffix code
None: msec
US: μsec
MS: msec
S: sec

■ Initial setting Calculated value when AUTO is selected for SWT

■ Example
SWT␣1S
SWT␣20ØMS

TDLY

TDLY Delay Time

■ Function Sets the delay time from the point where trace time trigger occurs.

Header	Program command	Query	Response
TDLY	TDLY␣t	TDLY?	t t=−1000000000 to 65500 Transfers the data without suffix code as if represented in units of μsec

■ Value of t −1000 sec to 65.5 msec

■ Suffix code
None: msec
US: μsec
MS: msec
S: sec

■ Initial setting Ø: 0 sec

■ Example TDLY␣20ØMS

TEXPAND Time Expand

■ Function Turns ON or OFF the expand functions of trace time.

Header	Program command	Query	Response
TEXPAND	TEXPAND␣sw sw=ON, 1, OFF, 0	TEXPAND?	sw sw=ON, OFF

■ Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code None

■ Initial setting OFF

■ Example TEXPAND␣ON

TM Trigger

■ Function Sets the trigger switch/trigger source (same function as TRG).
This command allows both the trigger switch and the trigger source to be set.

Header	Program command	Query	Response
TM	TM␣a	TM?	a a=FREE, VID, LINE, EXT, TV

■ Value of a
FREE: FREERUN
VID: VIDEO
LINE: LINE
EXT: EXT
TV: TV

■ Suffix code None

■ Initial setting FREE: FREERUN

■ Example TM␣FREE

TMMD

TMMD Trace Time Storage Mode

■ Function Selects the mode for processing the trace TIME waveform.

Header	Program command	Query	Response
TMMD	TMMD␣a a=0 to 5	TMMD?	TMMD␣a a=0 to 5

■ Value of a
Ø: NORMAL
1: MAX HOLD
2: AVERAGE
3: MIN HOLD
4: CUMULATIVE
5: OVER WRITE

■ Suffix code None

■ Initial setting Ø: NORMAL

■ Example TMMD␣Ø

TMWR

TMWR Trace Time Write Switch

■ Function Controls writing the waveform to the trace TIME.

Header	Program command	Query	Response
TMWR	TMWR␣sw sw=ON, 1, OFF, 0	TMWR?	TMWR␣sw sw=ON, OFF

■ Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code None

■ Initial setting ON: ON

■ Example TMWR␣ON

TRG Trigger

■ Function

Sets the trigger switch/trigger source (same function as TM).
This command allows both the trigger switch and the trigger source to be set.

Header	Program command	Query	Response
TRG	TRG␣a a=0 to 3, 6	TRG?	TRG␣a a=0 to 3, 6

■ Value of a

Ø: FREERUN
1: VIDEO
2: LINE
3: EXT
6: TV

■ Suffix code

None

■ Initial setting

Ø: FREERUN

■ Example

```
TRG␣Ø
```


TRGLVL Trigger Level

■ Function

Sets the threshold level of the trigger for starting the sweep when trigger source = VIDEO, EXT (Input) are selected

Header	Program command	Query	Response
TRGLVL	TRGLVL␣ℓ	TRGLVL?	ℓ

■ Value of ℓ

−10.0 to +10.0 (0.1 Step) .... when the trigger source is EXT (Input1) (V unit)
−100 to +100 (1 Step) ..... when trigger source is VIDEO (% unit)

■ Suffix code

when trigger source is VIDEO None

when the trigger source is EXT None: V
V: V

■ Initial setting

Value of ℓ = 0.0

■ Example

```
TRGLVL␣-1Ø.Ø
TRGLVL␣9.9
```

TRGS

TRGS Trigger Switch

■ Function Switches the trigger switch to Free run or Triggered.

Header	Program command	Query	Response
TRGS	TRGS␣sw sw=FREE, TRGD	TRGS?	SW sw=FREE, TRGD

■ Value of sw FREE: FREERUN
TRGD: TRIGGERED

■ Suffix code None

■ Initial setting FREE: FREERUN

■ Example TRGS␣FREE

TRGSLP

TRGSLP Trigger Slope

■ Function Selects the positive or negative leading edge of the trigger when trigger source is VIDEO or EXT mode.

Header	Program command	Query	Response
TRGSLP	TRGSLP␣sw	TRGSLP?	SW sw=RISE, FALL

■ Value of sw RISE: Positive leading edge
FALL: Negative leading edge

■ Suffix code None

■ Initial setting RISE: Positive leading edge

■ Example TRGSLP␣RISE

TRGSOURCE Trigger Source

■ Function Selects the trigger source. Trigger switch setting is not changed by this command.

Header	Program command	Query	Response
TRGSOURCE	TRGSOURCE␣sw	TRGSOURCE?	sw sw = VID, LINE, EXT, TV

■ Value of sw
VID: VIDEO
LINE: LINE
EXT: EXT
TV: TV

■ Suffix code None

■ Initial setting VID: VIDEO

■ Example TRGSOURCE␣VID

TS Take Sweep

■ Function Executes single sweep synchronously (same function as SWP).

Header	Program command	Query	Response
TS	TS	———	———

■ Example TS

TSP

TSP Time Span

■ Function Sets the span of trace time.

Header	Program command	Query	Response
TSP	TSP␣t	TSP?	t t=50 to 1000000000 Transfers the data without suffix code as if represented in units of μsec

■ Value of t 50 μsec to 1000 sec

■ Suffix code None: msec
US: μsec
MS: msec
S: sec

■ Initial setting 200 msec

■ Example TSP␣100
TSP␣100S

TVLINE

TVLINE TV (H-Sync: line)

■ Function Sets the number of lines used in the TV horizontal synchronous signal.

Header	Program command	Query	Response
TVLINE	TVLINE␣a	TVLINE?	a a=5 to 310

■ Value of a 9 to 262 (NTSC EVEN)
10 to 263 (NTSC ODD)
5 to 310 (PAL EVEN)
6 to 310 (PAL ODD)

■ Suffix code None

■ Initial setting a=10

■ Example TVLINE␣10

TVSFRM TV Synchronizing Signal

■ Function Sets the TV synchronous signal when TV is selected for trigger source.

Header	Program command	Query	Response
TVSFRM	TVSFRM␣sw	TVSFRM?	SW sw=VERTICAL, EVEN, ODD

■ Value of sw
VERTICAL: VERTICAL
EVEN: H-EVEN
ODD: H-ODD

■ Suffix code None

■ Initial setting VERTICAL: VERTICAL

■ Example TVSFRM␣VERTICAL

TVSTND TV Type

■ Function Sets the TV broadcasting system when TV is selected for trigger source.

Header	Program command	Query	Response
TVSTND	TVSTND␣sw	TVSTND?	SW sw=PAL, NTSC

■ Value of sw
PAL: PAL
NTSC: NTSC

■ Suffix code None

■ Initial setting NTSC: NTSC

■ Example TVSTND␣NTSC

TZONE

TZONE Expand Zone

■ Function Switches the time expand (magnified display) mode to ON or OFF.

Header	Program command	Query	Response
TZONE	TZONE␣SW sw=ON, 1, OFF, 0	TZONE?	SW sw=ON, OFF

■ Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code None

■ Initial setting OFF: OFF

■ Example TZONE␣ON

TZSP

TZSP Expand Zone Span

■ Function Sets the zone for expanding the time expand (magnified display).

Header	Program command	Query	Response
TZSP	TZSP␣t	TZSP?	t t=50 to 1000000000 Transfers the data without suffix code as if represented in units of μsec

■ Value of t 50 μsec to 1000 sec

■ Suffix code
None: msec
US: μsec
MS: msec
S: sec

■ Initial setting 200 msec

■ Example TZSP␣1ØMS

TZSTART Expand Zone Start

■ Function Sets the start time of time expand (magnified display).

Header	Program command	Query	Response
TZSTART	TZSTART␣t	TZSTART?	t t=−1000000000 to 65500 Transfers the data without suffix code as if represented in units of μsec

■ Value of t −1000 sec to 65.5 msec

■ Suffix code None: msec
US: μsec
MS: msec
S: sec

■ Initial setting 0 sec

■ Example TZSTART␣10MS

UCL? Query Uncal Status

■ Function Reads out the UNCAL status.

Header	Program command	Query	Response
UCL?	———	UCL?	UCL␣a a=0, 1

■ Value of a 0: NORMAL
1: During UNCAL

■ Example UCL?

UNC

UNC Uncal Display ON/OFF

■ Function Sets whether 'UNCAL' is displayed or not when UNCAL has occurred.

Header	Program command	Query	Response
UNC	UNC␣SW sw=ON, 1, OFF, 0	UNC?	UNC␣SW sw=ON, OFF

■ Value of sw
ON: ON
1: ON
OFF: OFF
Ø: OFF

■ Suffix code None

■ Initial setting ON: ON

■ Example UNC␣ON

UNT

UNT Unit for Log Scale

■ Function Sets one of the display unit systems in LOG scale mode.

Header	Program command	Query	Response
UNT	UNT␣a a=0 to 4	UNT?	UNT␣a a=0 to 4

■ Value of a
Ø: dBm
1: dBμV
2: dBmV
3: V
4: dBμV (emf)
5: W

■ Suffix code None

■ Initial setting Ø: dBm

■ Example UNT␣Ø

VAVG Average

■ Function Sets averaging to ON, OFF, or number of processing.

Header	Program command	Query	Response
VAVG	VAVG␣sw VAVG␣a	VAVG?	a a=2 to 256

■ Value of a
Ø: dBm
1: dBμV
2: dBmV
3: V
4: dBμV (emf)
5: W

■ Suffix code None

■ Initial setting Ø: dBm

■ Example
VAVG␣ON
VAVG␣128

VB Video Band Width

■ Function Sets the video bandwidth (same function as VBW).

Header	Program command	Query	Response
VB	VB␣f VB␣a	VB?	f f=1 to 3000000 or OFF Transfers the data without suffix code as if represented in units of Hz

■ Value of f
1 Hz to 3 MHz (1/3 sequence)
OFF: OFF

■ Value of a
AUTO: AUTO
UP: VBW UP
DN: VBW DOWN

■ Suffix code
f: None: Hz (10^0) MHZ, MZ: MHz (10^6)
HZ: Hz (10^0) GHZ, GZ: GHz (10^9)
KHZ, KZ: kHz (10^3)
a: None

■ Initial setting Calculated value when VBW is selected for AUTO

■ Example VB␣300HZ

VBCOUPLE

VBCOUPLE Couple Mode

■ Function Sets the coupled functions (RBW/VBW/SWT) commonly or independently between frequency domain or time domain.

Header	Program command	Query	Response
VBCOUPLE	VBCOUPLE␣sw	VBCOUPLE?	sw sw=COM, IND

■ Value of sw
COM: Common setting
IND: Independent setting

■ Suffix code None

■ Initial setting COM: Common setting (provided the unit already registered is not initialized)

■ Example VBCOUPLE␣COM

VBR

VBR VBW/RBW ratio

■ Function Sets the ratio of video bandwidth and resolution bandwidth when VBW is selected for AUTO.

Header	Program command	Query	Response
VBR	VBR␣r	VBR?	r r=0.0001 to 100

■ Value of r 0.0001 to 100 (1/3 sequence)

■ Suffix code None

■ Initial setting Trace FREQ VBW/RBW RATIO = 1
Trace TIME VBW/RBW RATIO = 1

■ Example VBR␣1

VBW Video Band Width

■ Function Sets the video bandwidth.

Header	Program command	Query	Response
VBW	VBW␣a a=0 to 14	VBW?	VBW␣a a=0 to 14

■ Value of a
Ø: 1 Hz 8: 3 Hz
1: 10 Hz 9: 30 Hz
2: 100 Hz 1Ø: 300 Hz
3: 1 kHz 11: 3 kHz
4: 10 kHz 12: 30 kHz
5: 100 kHz 13: 300 kHz
6: OFF 14: 3 MHz
7: 1 MHz

■ Suffix code None

■ Initial setting Calculated value when VBW is selected for AUTO

■ Example VBW␣3

VIEW View

■ Function Stops writing the waveform data.

Header	Program command	Query	Response
VIEW	VIEW␣tr	———	———

■ Value of tr
TRA: Trace A (FREQ)
TRTIME: Trace TIME

■ Suffix code None

■ Example VIEW␣TRB

(Blank)

SECTION 7
SAMPLE PROGRAMS

This section gives some examples of the N_{88}-Basic program that controls the MS8604A from the NEC-PC9800 personal computer which is used as a controller.

TABLE OF CONTENTS

7.1 Precautions on Creating the GPIB Program 7-3

7.2 Sample Programs 7-4

(1) Initializing MS8604A 7-4

(2) Reading the frequency and level at marker point 7-5

(3) Reading the modulation precision 7-7

(4) Reading the I-Q data 7-8

(5) Reading marker point levels 7-13

(6) Measuring the occupied frequency bandwidth 7-14

(7) Measuring the adjacent channel leakage power 7-15

(8) Measuring spurious harmonics 7-16

(Blank)

7.1 Precautions on Creating the GPIB Program

Note the following points when writing GPIB control programs.

No.	Precaution	Description
1	Be sure to initialize each device.	There may be a number of the state in which each device is not proper to be actually used due to operation on its own panel or execution of other programs. It is necessary to using individual devices with a prescribed condition resulting from initializing them. Execute the following. ① Initializing the interface functions (**ISET IFC**) ② Initializing message exchange functions of each device (**WBYTE &H3F, &H14**) ③ Initializing the functions proper to each device (**PRE, INI, or *RST**)*
2	Turn the device to the remote state of RWLS (Remote With Lockout State).	In a simple remote state, pressing [**Local**] turns the device to the local state. Pressing a panel key in this moment causes device's automatic measurement to function improperly, thus measurement data are likely to turn out unreliable. Set the device to the locally locked out state with **WBYTE &H3F, &H11** to prevent it from returning to the local state. (Turn every device to the locally controlled state with **WBYTE &H3F, <listener address>, [secondary address], &H01.**)
3	Do not send any command (related to the device) other than the **INPUT @** statement immediately after sending a query.	If MLA is received when a command other than the **INPUT @** statement is sent to the controller before the response to a query is read, the output buffer is cleared, and the response message disappears. For this reason, write the **INPUT @** statement in immediate succession to a query.
4	Create a program that avoids an exception processing of the protocol	Avoid stoppage of execution (caused by an error) by means of providing a program with exception-processing section against exceptions that can be foreseen.
5	Confirm the interface functions of each device (subset).	Execution of program does not advance if necessary subset (s) has (have) not been prepared in the device. Be sure to confirm the subset (s) of each device. Also confirm that each device complies with IEEE 488.2.

7.2 Sample Programs

(1) Initializing MS8604A

<Example 1 > Initializes MS8604A

```
10 '-----------------------------
20 ' MS8604A GPIB SAMPLE PROGRAM
30 ' INITIALIZE
40 '-----------------------------
50 ISET IFC ..... Initializes the interface function
60 ISET REN ..... Sets remote enable to true
70 CMD DELIM=0 ..... Selects CR + LF as the delimiter
80 LET SPA=1 ..... Assigns MS8604A address to variable SPA
90 PRINT @SPA;"INI" ..... Initializes MS8604A
100 END
```

Separate volume " Panel Operation Appendix B " describes the parameters initialized by the above program.

There is a '*RST ' command in another GPIB command for executing initialization. The '*RST ' command is used to execute initialization over a wider range. For the range of initialization level, see SECTION 5. The usage of the 'IP' and 'PRE' commands are identical to the 'INI' command.

For general usage of INI and *RST, first initialize the MS8604A device functions with the IP or INI command, then use the program commands to set only the functions to be changed. This prevents the MS8604A from being controlled while unnecessary functions are set.

(2) Reading the frequency and level at marker point

<Example 2> Sets the center frequency to 500 MHz and span to 10 MHz, then displays the frequency and level reading at the peak point on the controller screen when a signal to be measured is received.

```
10 '------------------------------
20 ' MS8604A GPIB SAMPLE PROGRAM
30 ' OUTPUT MKR FREQ&LEVEL
40 '------------------------------
50 ISET IFC
60 ISET REN
70 CMD DELIM=0
80 LET SPA=1
90 PRINT @SPA;"INI"
95 PRINT @SPA;"PNLMD SPECT"  ..... Sets to spectrum mode
100 PRINT @SPA;"CNF 500MHZ"  ..... Sets the center frequency
110 PRINT @SPA;"SPF 10MHZ"   ..... Sets the frequency span
120 PRINT @SPA;"SWP"         ..... Executes single sweep
130 PRINT @SPA;"PCF"         ..... PEAK→CF
140 PRINT @SPA;"PRL"         ..... PEAK→REF
150 PRINT @SPA;"MKS 0"       ..... Peak search
160 PRINT @SPA;"MKF?"        ..... Queries reading frequency at the marker point
170 INPUT @SPA;FREQ          ..... Reads the frequency at the marker point
180 PRINT @SPA;"MKL?"        ..... Queries reading level at the marker point
190 INPUT @SPA;LEVEL         ..... Reads the level at the marker point
200 PRINT USING "MARKER  FREQ=####.###MHz";FREQ/1E+06
210 PRINT USING "        LEVEL=####.## dBm";LEVEL
220 END
```

The center frequency and frequency span are set at line 100 and line 110 respectively. The SWP sweep command at line 120 does not execute the next message unless the sweep is completed. This command thus prevents the peak search and other program lines from being executed before the sweep is completed.

The PCF and PRL commands at lines 130 and 140 operate as follows: the former sets the peak point on the screen to the center frequency, and the latter sets its peak level center frequency to the reference level.

The " MKF? " and " MKL? " at lines 160 and 180 query the frequency and level at the marker point respectively, and the data is read with the INPUT@ statement on the next line. If MLA (My Listen Address) is received when a command other than the INPUT@ statement is sent before the response to a query is read, the output buffer is cleared, and the response message is deleted. For this reason, write the INPUT@ statement immediately after a query.

[Sending data]

If the frequency and level at the peak point is 501.251 MHz and −15.53 dBm respectively,

■ FREQ

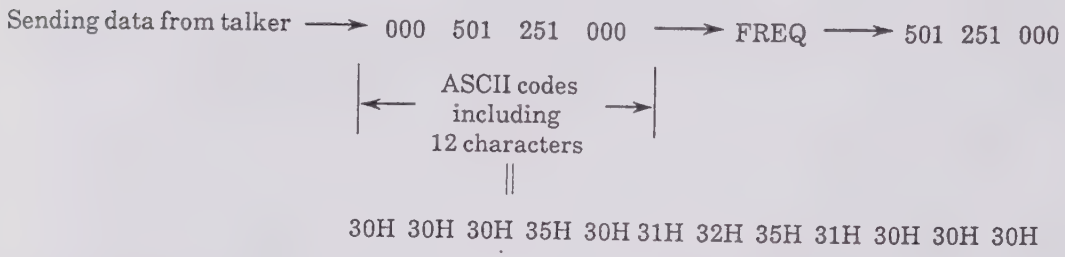

■ LEVEL

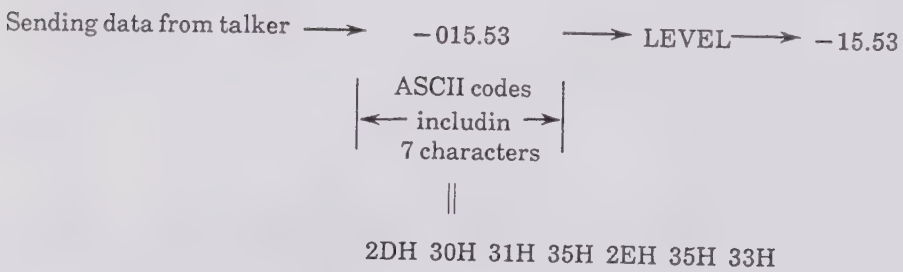

Program execution result of <Example 2>

```
MARKER  FREQ=501.251MHz
        LEVEL=-15.53 dBm
```

(3) Reading the modulation precision

<Example 3> Reads vector and peak vector errors, then display the read errors on the controller screen.

```
100 '------------------------------
110 ' MS8604A GPIB SAMPLE PROGRAM
120 ' OUTPUT VECTOR ERROR
130 '------------------------------
140 ISET IFC
150 ISET REN
160 CMD DELIM=0
170 SPA=1
180 '
190 PRINT @SPA;"INI"
200 PRINT @SPA;"PNLMD TESTER"
210 PRINT @SPA;"SYS PHS"
220 PRINT @SPA;"MEAS MODANAL"
230 PRINT @SPA;"SWP" ..... Executes measurement once.
240 '
250 PRINT @SPA;"VECTERR?" ..... Vector error
260 INPUT @SPA;VSTS,VERR
270 PRINT @SPA;"PVECTERR?" ..... Peak vector error
280 INPUT @SPA;PVSTS,PVERR
290 '
300 PRINT USING "RMS vector error  = ##.## % (rms)";VERR
310 PRINT USING "Peak vector error = ##.## %      ";PVERR
320 END
```

Lines 200 and 210 switch the system to the PHS system in transmitter tester mode. (If always using the device as a transmitter tester, this switching is not necessary). Line 220 switches the screen to the modulation analysis screen.

Lines 250 and 270 read the vector and peak vector errors. Two data items separated by a comma (,) are output as the response data to the query command. The first data item is the measurement result status. If this value is 0, it indicates normal termination (see to the " GPIB Command Reference "). The second data item is the measurement result.

(4) Reading the I-Q data

<Example 4-1> Reads all data items of the I-Q constellation.

```
100 '------------------------------
110 ' MS8604A GPIB SAMPLE PROGRAM
120 ' OUTPUT I/Q DATA (ASCII)
130 '------------------------------
140 ISET IFC
150 ISET REN
160 CMD DELIM=0
170 SPA=1
180 NUM=438 ..... Number of data items to be read
190 DIM TRACE(1,NUM) ..... Declaration of array variable TRACE ( )
200 '
210 PRINT @SPA;"INI"
220 PRINT @SPA;"PNLMD TESTER"
230 PRINT @SPA;"SYS PHS"
240 PRINT @SPA;"MEAS CONSTEL"
250 PRINT @SPA;"BIN 0" ..... Sets to the data to be read to ASCII.
260 PRINT @SPA;"SWP" ..... Executes measurement once.
270 '
280 FOR I=0 TO 1
290 FOR J=0 TO NUM-1
300     PRINT @SPA;"XMC? "+STR$(I)+","+STR$(J)+",1"
                                    ..... Data query
310     INPUT @SPA;TRC$ ..... Data reading
320     TRACE(I,J)=VAL(TRC$) ..... ASCII to numeric data conversion
330 NEXT J
340 NEXT I
350 '
360 FOR J=0  TO NUM-1
370     PRINT USING "##.####,##.####";TRACE(0,J)/10000,TRACE(1
,J)/10000
380 NEXT J
390 END
```

"BIN␣0" in line 250 is the command that converts read data into ASCII format.

"XMA?", "XMB?", "XMC?", "XMD?", "XME?", and "XMT?" output data in ASCII or binary format. Example 4-2 shows an example of reading binary format data.

<Example 4-2> Reads the I/Q data in binary format.

```
100 '------------------------------
110 ' MS8604A GPIB SAMPLE PROGRAM
120 ' OUTPUT I/Q DATA (BINARY)
130 '------------------------------
140 ISET IFC
150 ISET REN
160 CMD DELIM=0
170 SPA=1
180 NUM=438 ..... Number of read data items
190 DIM TRACE(1,NUM)
200 '
210 PRINT @SPA;"INI"
220 PRINT @SPA;"PNLMD TESTER"
230 PRINT @SPA;"SYS PHS"
240 PRINT @SPA;"MEAS CONSTEL"
250 PRINT @SPA;"BIN 1" ..... Sets the read data to binary format.
260 PRINT @SPA;"TRM 1" ..... Sets the terminator to CR + LF.
270 PRINT @SPA;"SWP" ..... Executes measurement once.
280 '
290 FOR I=0 TO 1
300 PRINT @SPA;"XMC? "+STR$(I)+",0,"+STR$(NUM)
                                    ..... Data query
310 WBYTE &H3F,&H5F,&H20,&H41;
                          .. Specifies the PC9801 to the talker and MS8604A to the listener.
320 FOR J=0 TO NUM-1
330     RBYTE ;UPRBYTE,LWRBYTE ..... Receives the data every two-byte units.
340     TRACE(I,J)=UPRBYTE*256+LWRBYTE ... Converts the data to decimal data.
350     IF UPRBYTE>=128 THEN TRACE(I,J)=TRACE(I,J)-65536!
                                    ..... Converts negative data.
360 NEXT J
370 RBYTE ;DMY1,DMY2 ..... Terminator receiving
380 WBYTE &H3F,&H5F; ..... Listener and talker release
390 NEXT I
400 '
410 FOR J=0  TO NUM-1
420     PRINT USING "##.####,##.####";TRACE(0,J)/10000,TRACE(1
,J)/10000
430 NEXT J
440 END
```

The " BIN_1 " at line 250 specifies the data format as the binary format. The terminator indicating that the last data byte transmission is completed is set to CR + LF at line 260. The data query in line 300 is performed after measurement is executed once in line 270. At line 310, the PC9801 (address 0) is specified as a listener, and the MS8604A (address 1) as a talker. At line 330, the 2-byte binary data is read by the PC9801 in sequence from the high-order byte to the low-order byte. At line 340, the 2-byte binary data is converted into decimals to assign them to variable TRACE (1). Line 350 allows data to be correctly read even if the data is negative. Statements from the FOR statement to the NEXT statement in lines 320 to 360 are executed repeatedly for each read data item.

At line 370, the terminators transferred immediately after the last data byte transmission is completed are assigned to dummy variables DMY1 and DMY2. This prevents the CR+LF (LF for TRM_0) terminators from being assigned elsewhere. Although two variables DMY1 and DMY2 are used here, one variable is used if the terminator is LF. Line 380 is used to release the talker and listener.

Statements from the FOR statement to the NEXT statement in lines 290 to 390 are executed twice to read the I/Q data.

[Interface message at line 310]

```
WBYTE   &H3F,  &H5F,  &H20,  &H41 ;
          └──┘   └──┘   └──┘   └──┘
          UNL    UNT    MLA    MTA
```

UNL=Unlisted : Specifies all devices so that the listener status can be released.

UNT=Untalk : Specifies all devices so that the talker status can be released.

MLA=My Listen Address : If a device receives the listener address code (listener address command −MLA) corresponding to the address (address number) specified for the device (device and controller), it becomes a listener.

The &H20 listener address code specifies a device with address number 0 as listener.

MTA=My Talk Address : If a device receives the talker address code (talker address command −MTA) corresponding to the address (address number) specified for the device (device and controller), it becomes a talker.

The &H41 talker address code specifies a device with address number 1 as talker.

[Transferring 2-byte binary data]

Two-byte binary data can lie in the range of the 65536 integers from −32768 to 32767 as shown below, and each is sent out in sequence from the high-order byte to the low-order byte.

16-Bit Binary	With Sign	No Sign
1000000000000000	−32768	32768
1000000000000001	−32767	32769
1000000000000010	−32766	32770
1111111111111101	−3	65533
1111111111111110	−2	65534
1111111111111111	−1	65535
0000000000000000	0	0
0000000000000001	1	1
0000000000000010	2	2
0000000000000011	3	3
0111111111111101	32765	32765
0111111111111110	32766	32766
0111111111111111	32767	32767

Sign bit : Bit 15 (MSB) is used

Integer bits : Bits 0 through 14 are used. Thus, 16 bits (2 bytes) are used.

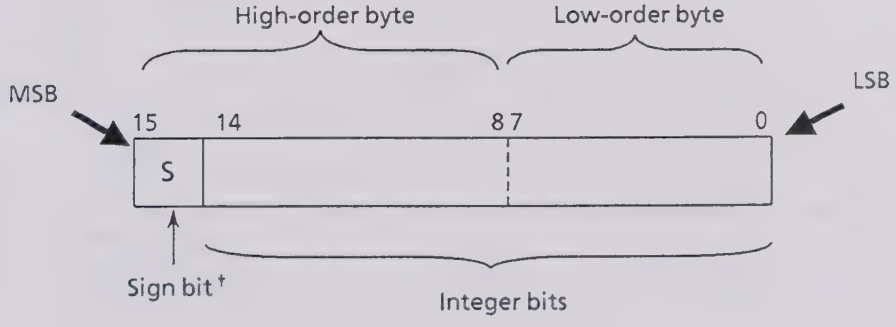

Internal Expression of 2-byte Binary Data

† When a negative integer is stored in a numeric variable, its MSB is set to 1 to indicate that it is negative. The negative value is also stored in a numeric variable as a two's-complement.

The transfer of integer 16706 as ASCII data and as binary data is compared below. 5 bytes are necessary for ASCII, whereas only 2 bytes are necessary for binary and no data format conversion is required. Thus, the latter is often used for high speed transfer.

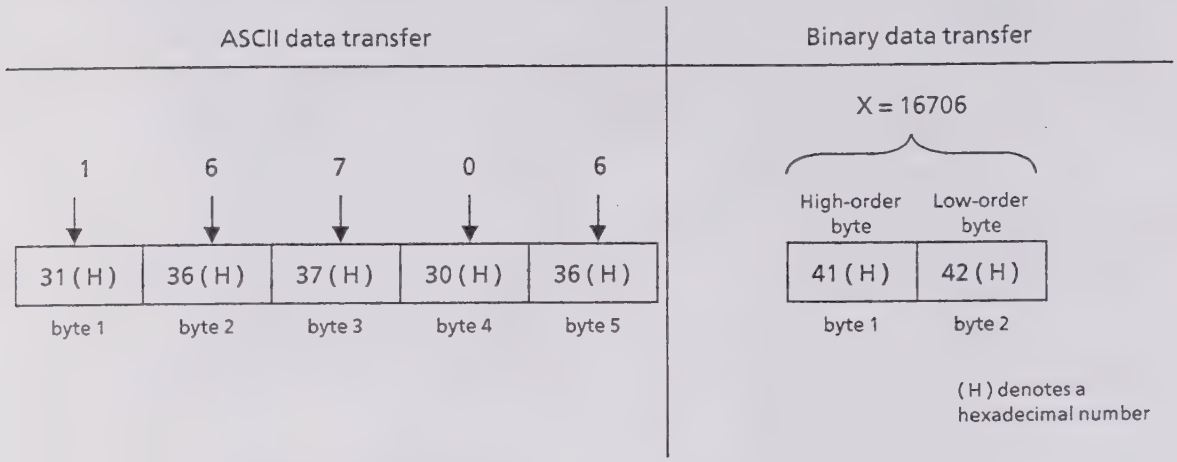

$$16706\,(D) = 4\times16^{3} + 1\times16^{2} + 4\times16^{1} + 2\times16^{0}$$

Binary notation

	High-order byte								Low-order byte							
bit	15	14	13	12	11	10	9	8	7	6	5	4	3	2	1	0
X = 16706	0	1	0	0	0	0	0	1	0	1	0	0	0	0	1	0

(Transfer sequence) First byte → Second byte

bit	7	6	5	4	3	2	1	0
	0	1	0	0	0	0	0	1
Second byte	0	1	0	0	0	0	1	0

High-order byte = 41 (H)

Low-order byte = 42 (H)

(5) Reading marker point levels

<Example 5> Reads levels of the first and second symbols.

```
100 '------------------------------
110 ' MS8604A GPIB SAMPLE PROGRAM
120 ' OUTPUT RF POWER(MARKER)
130 '------------------------------
140 ISET IFC
150 ISET REN
160 CMD DELIM=0
170 SPA=1
180 '
190 PRINT @SPA;"INI"
200 PRINT @SPA;"PNLMD TESTER"
210 PRINT @SPA;"SYS PHS"
220 PRINT @SPA;"MEAS RFPWR"
230 PRINT @SPA;"LVLREL ON" ..... Sets this item to a relative value.
240 PRINT @SPA;"SWP" ..... Executes measurement once.
250 '
260 PRINT @SPA;"MKRS 1" ..... Sets the marker to the first symbol.
270 PRINT @SPA;"MKL?" ..... Marker level query
280 INPUT @SPA;MKR1
290 PRINT @SPA;"MKRS 2" ..... Sets the marker to the second symbol.
300 PRINT @SPA;"MKL?" ..... Marker level query
310 INPUT @SPA;MKR2
320 '
330 PRINT USING "1 symbol = ###.## dB";MKR1
340 PRINT USING "2 symbol = ###.## dB";MKR2
350 END
```

Line 230 sets the relative value display. Lines 260 and 290 move the markers to the specified symbol locations.

Use this program to read the level change between symbols at the rising and falling edges of a burst.

(6) Measuring the occupied frequency bandwidth

<Example 6> Reads the mean value of 16 measurements in HIGH SPEED mode.

```
100 '------------------------------
110 ' MS8604A GPIB SAMPLE PROGRAM
120 ' OUTPUT OCC.BW
130 '------------------------------
140 ISET IFC
150 ISET REN
160 CMD DELIM=0
170 SPA=1
180 '
190 PRINT @SPA;"INI"
200 PRINT @SPA;"PNLMD TESTER"
210 PRINT @SPA;"SYS PHS"
220 PRINT @SPA;"MEAS OBW,HIGH"
230 PRINT @SPA;"*CLS" ..... Clears the status register.
240 PRINT @SPA;"AVR 16" ..... Sets the average count to 16.
250 PRINT @SPA;"STORAGE AVG" ..... Sets the average mode.
260 PRINT @SPA;"SWP" ..... Executes measurement once.
270 '
280 WHILE ENDSTS<>17 ..... Repeats processing until averaging terminates.
290 PRINT @SPA;"ESR2?" ..... END-STATUS query
300 INPUT @SPA;ENDSTS
310 WEND
320 '
330 PRINT @SPA;"OCCBW?"
340 INPUT @SPA;OSTS,OCCBW
350 '
360 PRINT USING "Occupied bandwidth = ###.# kHz";OCCBW/1000
370 END
```

Line 230 clears the status registers. Line 240 sets the average count to 16 and line 250 switches the mode to the average mode. After SWP in line 260 executes measurement once, the program executes measurement for the average count, then terminates.

Lines 280 to 310 check the average count.

(7) Measuring the adjacent channel leakage power

<Example 7> Reads the mean power in HIGH SPEED mode and displays the read power on the controller screen.

```
100 '------------------------------
110 ' MS8604A GPIB SAMPLE PROGRAM
120 ' OUTPUT ADJ.CH
130 '------------------------------
140 ISET IFC
150 ISET REN
160 CMD DELIM=0
170 SPA=1
180 '
190 PRINT @SPA;"INI"
200 PRINT @SPA;"PNLMD TESTER"
210 PRINT @SPA;"SYS PHS"
220 PRINT @SPA;"MEAS ADJ,HIGH"
                    ..... Sets the adjacent channel leakage power to HIGH SPEED.
230 PRINT @SPA;"UNIT DBM" ..... Sets the units to dBm.
240 PRINT @SPA;"SWP" ..... Executes measurement once.
250 '
260 PRINT @SPA;"MEANPWR? LOW2,DBM"
                    ..... Lower next adjacent channel leakage power query
270 INPUT @SPA;L2STS,LOW2
280 PRINT @SPA;"MEANPWR? LOW1,DBM"
                    ..... Lower adjacent channel leakage power query
290 INPUT @SPA;L1STS,LOW1
300 PRINT @SPA;"MEANPWR? UP1,DBM"
                    ..... Upper adjacent channel leakage power query
310 INPUT @SPA;U1STS,UP1
320 PRINT @SPA;"MEANPWR? UP2,DBM"
                    ..... Upper next adjacent channel leakage power query
330 INPUT @SPA;U2STS,UP2
340 '
350 PRINT "Adjacent channel power"
360 PRINT USING "     Mean power  (-900kHz) = ###.## dBm";LOW2
370 PRINT USING "                 (-600kHz) = ###.## dBm";LOW1
380 PRINT USING "                 ( 600kHz) = ###.## dBm";UP1
390 PRINT USING "                 ( 900kHz) = ###.## dBm";UP2
400 END
```

(8) Measuring spurious harmonics

<Example 8> Reads the spurious harmonics in SPOT mode and displays them on the controller screen.

```
100 '------------------------------
110 ' MS8604A GPIB SAMPLE PROGRAM
120 ' OUTPUT SPURIOUS
130 '------------------------------
140 ISET IFC
150 ISET REN
160 CMD DELIM=0
170 SPA=1
180 '
190 PRINT @SPA;"INI"
200 PRINT @SPA;"PNLMD TESTER"
210 PRINT @SPA;"SYS PHS"
220 PRINT @SPA;"MEAS SETTABLE" ..... Sets the frequency setting screen.
230 PRINT @SPA;"SPUFREQ HRM" ..... Set up to the fifth harmonic.
240 PRINT @SPA;"MEAS SPURIOUS,SPOT"
                          ..... Sets spot measurement of the spurious harmonics.
250 PRINT @SPA;"UNIT DBM"
260 PRINT @SPA;"SWP" ..... Executes measurement once.
270 '
280 PRINT @SPA;"SPULVL? F1" ..... Spurious harmonics query
290 INPUT @SPA;F1STS,F1LVL
300 PRINT @SPA;"SPULVL? F2" ..... Spurious harmonics query
310 INPUT @SPA;F2STS,F2LVL
320 PRINT @SPA;"SPULVL? F3" ..... Spurious harmonics query
330 INPUT @SPA;F3STS,F3LVL
340 PRINT @SPA;"SPULVL? F4" ..... Spurious harmonics query
350 INPUT @SPA;F4STS,F4LVL
360 '
370 PRINT "Spurious emissions"
380 PRINT USING "       F1 = ###.## dBm";F1LVL
390 PRINT USING "       F2 = ###.## dBm";F2LVL
400 PRINT USING "       F3 = ###.## dBm";F3LVL
410 PRINT USING "       F4 = ###.## dBm";F4LVL
420 END
```

Line 220 switches to the frequency setting screen and line 230 sets the frequency for the spurious harmonics two to five times higher than the frequency on the parameter setting screen.

Line 240 switches to the spurious harmonics measurement screen. Lines 280 to 350 examine the spurious harmonics.

SECTION 8
WAVEFORM DATA STORAGE FORMAT

This section describes the storage format of waveform data fetched by the PTA or external computer. The use examples are described in NEC 9800 series N_{88}-BASIC.

TABLE OF CONTENTS

8.1 Notes on Fetching the Waveform Data 8-3

8.2 Waveform Data Storage Format 8-4

(1) XMA, XMT (Spectrum screen) 8-4

(2) XMB (STANDARD method of the occupied frequency bandwidth and adjacent channel leakage power measurement screen) 8-5

(3) XMC (Constellation screen) 8-6

(4) XMD (Power measurement screen) 8-7

(5) XME (HIGH SPEED method of the occupied frequency bandwidth screen) 8-8

(Blank)

8.1 Notes on Fetching the Waveform Data

(1) Fetching screen

- The waveform data to be fetched needs to be displayed on the screen.
- Switch to SINGLE measurement mode before fetching the waveform data, and check that the measurement terminates. If CONTINUOUS measurement mode is set or measurement does not terminate, the correct data cannot be fetched.

(2) Response data

- When fetching two or more data items together, commas (,) are output as data separators.
- The query command format is designed so that it can fetch all data items together. However, the number of data items actually fetched depends on the restrictions of the PTA or external computer.

8.2 Waveform Data Storage Format

(1) XMA, XMT

a) Format

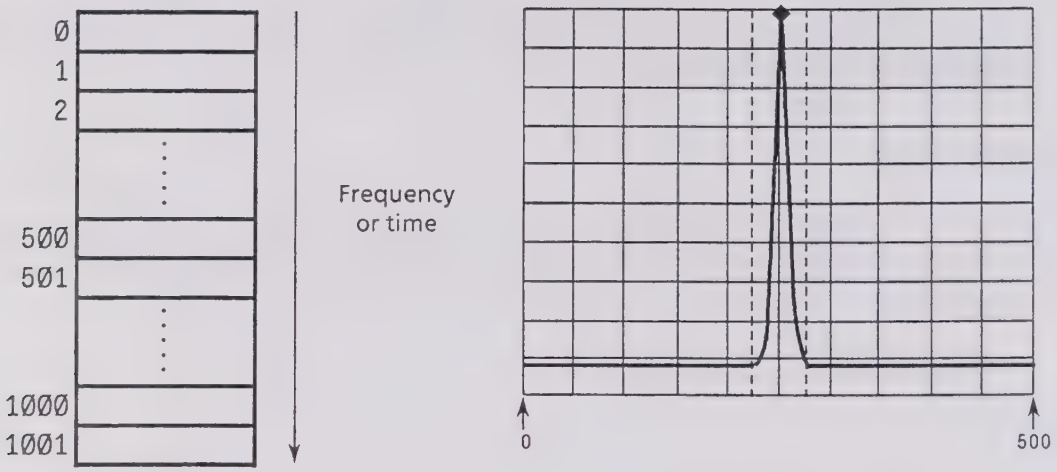

- The number of data items depends on the set data point value.

  In NORMAL mode: 501 points (0 to 500)
  In DOUBLE mode: 1002 points (0 to 1001)

- Correspondences to screen displays are as follows:

  In NORMAL mode: Waveform data Y_n is displayed as the nth data item on the screen.

  In DOUBLE mode: Waveform data $\frac{Y_{2n}+Y_{2n+1}}{2}$ is displayed as the nth data item on the screen.

b) Range

- In LOG scale mode: Displays an integer value in 0.01 dBm units (1 dBm = 100).
- In LIN scale mode: Displays $\frac{\text{Voltage value (V)}}{\text{Reference level (V)}} \times 10000$.

c) Use examples

```
PRINT␣@1;"XMA?␣Ø,1"
INPUT␣@1;LVL
```

(2) XMB

a) Format

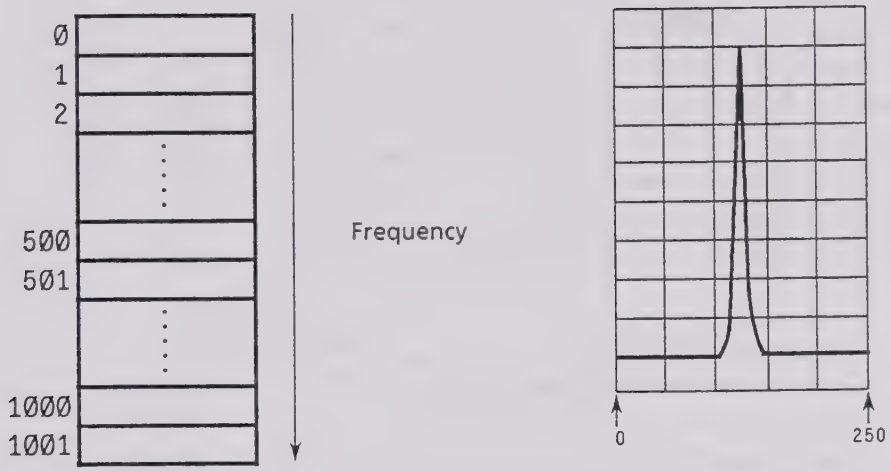

- The number of data items depends on the set data point value.

  In NORMAL mode: 501 points (0 to 500)
  In DOUBLE mode: 1002 points (0 to 1001)

- Correspondences to screen displays are as follows:

  In NORMAL mode: Waveform data $\frac{Y_{2n}+Y_{2n+1}}{2}$ is displayed as the nth data item on the screen.

  In DOUBLE mode: Waveform data $\frac{Y_{4n}+Y_{4n+1}+Y_{4n+2}+Y_{4n+3}}{4}$ is displayed as the nth data item on the screen.

b) Range

- Displays an integer value in 0.01 dBm units (1 dBm = 100).

c) Use examples

```
PRINT␣@1;"XMB␣1,2"
INPUT␣@1;LVL1,LVL2
```

(3) XMC

a) Format

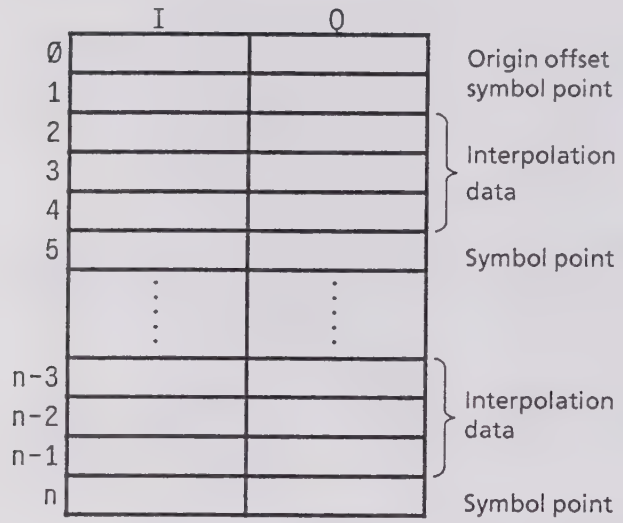

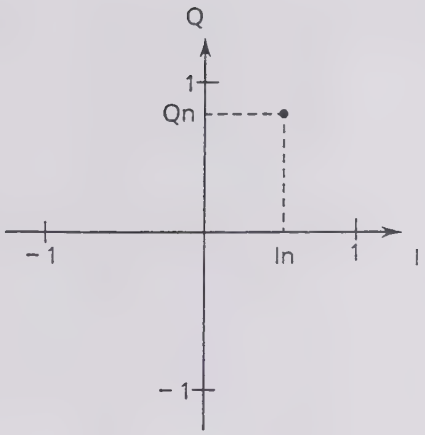

- Stored with the two-dimensional I-Q data.
- n depends on the measurement signal.
- Correspondences to screen displays are as follows (INTERPOLATION mode):

  NON: Dots represent symbol points (1, 5, ···, n).
  LINEAR: A symbol point is enclosed in a linear line frame (1−5− ···−n).
  4POINT: Dotted lines connect a symbol point and interpolation data (1−2−··· −n).

b) Range

- Displays an integer value in 0.0001 units (ideal signal 1 = 100000).

c) Use examples

- Fetch origin offsets.

```
PRINT␣@1;"XMC?␣Ø,Ø,1"
INPUT␣@1;IØ
PRINT␣@1;"XMC?␣1,Ø,1"
INPUT␣@1;QØ
```

(4) XMD

a) Format

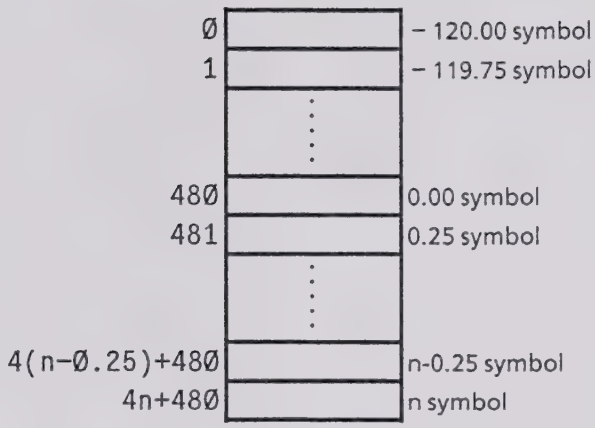

- n depends on the measuring system (PDC, PHS, 960, NADC, or 1020).
- The data corresponds to the horizontal axis scale of the screen display (RF POWER screen) in a one-to-one ratio.

b) Range

- Displays an integer value in 0.01 dBm units (1 dBm = 100).

c) Use examples

```
PRINT␣@1;"XMD?␣480,1"
INPUT␣@1;LVL
```

(5) XME

a) Format

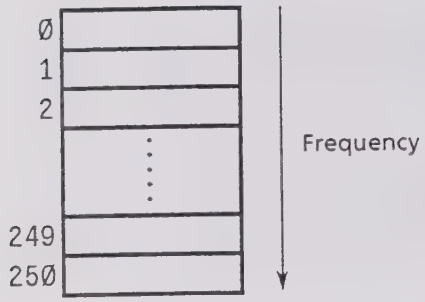

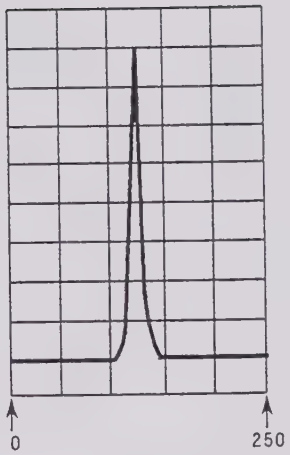

- The number of data items is fixed to 251 points.
- The data corresponds to the horizontal axis scale of the screen display (HIGH SPEED method of the occupied frequency bandwidth screen) in one-to-one ratio.

b) Range

- An integer in a 0.01 dBm unit (1 dBm = 100) represents the range.

c) Use examples

```
PRINT␣@1;"XME?␣Ø,Ø"
INPUT␣@1;LVL
```

APPENDIX A ASCII*CODE TABLE

BITS B4 B3 B2 B1	B7 B6 B5 = 0 0 0	0 0 1	0 1 0	0 1 1	1 0 0	1 0 1	1 1 0	1 1 1
	CONTROL		NUMBERS SYMBOLS		UPPER CASE		LOWER CASE	
0 0 0 0	0 NUL 0 0	20 DLE 10 16	40 SP 20 32	60 0 30 48	100 @ 40 64	120 P 50 80	140 ` 60 96	160 p 70 112
0 0 0 1	1 GTL SOH 1 1	21 LLO DC1 11 17	41 ! 21 33	61 1 31 49	101 A 41 65	121 Q 51 81	141 a 61 97	161 q 71 113
0 0 1 0	2 STX 2 2	22 DC2 12 18	42 " 22 34	62 2 32 50	102 B 42 66	122 R 52 82	142 b 62 98	162 r 72 114
0 0 1 1	3 ETX 3 3	23 DC3 13 19	43 # 23 35	63 3 33 51	103 C 43 67	123 S 53 83	143 c 63 99	163 s 73 115
0 1 0 0	4 SDC EOT 4 4	24 DCL DC4 14 20	44 $ 24 36	64 4 34 52	104 D 44 68	124 T 54 84	144 d 64 100	164 t 74 116
0 1 0 1	5 PPC ENO 5 5	25 PPU NAK 15 21	45 % 25 37	65 5 35 53	105 E 45 69	125 U 55 85	145 e 65 101	165 u 75 117
0 1 1 0	6 ACK 6 6	26 SYN 16 22	46 & 26 38	66 6 36 54	106 F 46 70	126 V 56 86	146 f 66 102	166 v 76 118
0 1 1 1	7 BEL 7 7	27 ETB 17 23	47 ' 27 39	67 7 37 55	107 G 47 71	127 W 57 87	147 g 67 103	167 w 77 119
1 0 0 0	10 GET BS 8 8	30 SPE CAN 18 24	50 (28 40	70 8 38 56	110 H 48 72	130 X 58 88	150 h 68 104	170 x 78 120
1 0 0 1	11 TCT HT 9 9	31 SPD EM 19 25	51) 29 41	71 9 39 57	111 I 49 73	131 Y 59 89	151 i 69 105	171 y 79 121
1 0 1 0	12 LF A 10	32 SUB 1A 26	52 * 2A 42	72 : 3A 58	112 J 4A 74	132 Z 5A 90	152 j 6A 106	172 z 7A 122
1 0 1 1	13 VT B 11	33 ESC 1B 27	53 + 2B 43	73 ; 3B 59	113 K 4B 75	133 [5B 91	153 k 6B 107	173 { 7B 123
1 1 0 0	14 FF C 12	34 FS IC 28	54 , 2C 44	74 < 3C 60	114 L 4C 76	134 \ 5C 92	154 l 6C 108	174 ¦ 7C 124
1 1 0 1	15 CR D 13	35 GS 1D 29	55 - 2D 45	75 = 3D 61	115 M 4D 77	135] 5D 93	155 m 6D 109	175 } 7D 125
1 1 1 0	15 SO E 14	36 RS 1E 30	56 . 2E 46	76 > 3E 62	116 N 4E 78	136 ^ 5E 94	156 n 6E 110	176 ~ 7E 126
1 1 1 1	17 SI F 15	37 US 1F 31	57 / 2F 47	77 UNL ? 3F 63	117 O 4F 79	137 UNT — 5F 95	157 o 6F 111	177 RUBOUT (DEL) 7F 127
	Address command	Universal command	Listen address		Talk address		Secondary address or command	

KEY

octal / hex

25	PPU
	NAK
15	21

GPIB code
ASCII character
decimal

* USA Standard Code for Information Interchange

Table of GPIB Interface Messages (extended)

Bits b7	0	0	0	0	0	0	0	1	1	1	1	1	1	1	1
Bits b6	0	0	1	1	0	0	1	1	0	0	1	1	0	0	1	1
Bits b5	0	1	0	1	0	1	0	1	0	1	0	1	0	1	0	1
b4 ↓	b3 ↓	b2 ↓	b1 ↓	COLUMN → / ROW ↓	0	① MSG	1	MSG	2	MSG	3	MSG	4	MSG	5	MSG	6	MSG	7	MSG
0	0	0	0	0	NUL		DLE		SP		0		@		P				p	
0	0	0	1	1	SOH	GTL	DC1	LLO	!		1		A		Q		a		q	
0	0	1	0	2	STX		DC2		"		2		B		R		b		r	
0	0	1	1	3	ETX		DC3		#		3		C		S		c		s	
0	1	0	0	4	EOT	SDC	DC4	DCL	$		4		D		T		d		t	
0	1	0	1	5	ENQ	PPC	NAK	PPU	%		5		E		U		e		u	
0	1	1	0	6	ACK		SYN		&		6		F		V		f		v	
0	1	1	1	7	BEL		ETB				7		G		W		g		w	
1	0	0	0	8	BS	GET	CAN	SPE	(		8		H		X		h		x	
1	0	0	1	9	HT	TCT	EM	SPD	)		9		I		Y		i		y	
1	0	1	0	A	LF		SUB		*		:		J		Z		j		z	
1	0	1	1	B	VT		ESC		+		;		K		[		k		{	
1	1	0	0	C	FF		FS		,		<		L		\		l		|	
1	1	0	1	D	CR		GS		-		=		M		]		m		}	
1	1	1	0	E	SO		RS		.		>		N		^		n		~	
1	1	1	1	F	SI		US		/		?	UNL	O		_	UNT	o		DEL	

Listener address (MTA) assigned to equipment

Listener address (MTA) assigned to equipment

Talker address (MTA) assigned to equipment

Talker address (MTA) assigned to equipment

Meaning is defined by PCG

Meaning is defined by PCG

Address command group (ACG)

Universal command group (UCG)

Listen address group (LAG)

Talk address group (TAG)

Primary command group (PGG)

Secondary command group (SCG)

Notes :
① MSG = INTERFACE MESSAGE (Sent by ATN of True: Low level.)
② b_1 = DI 01 ····· b_7 = DI 07 (b1 through b7 correspond to DIO1 to DIO7 sequence.)

GTL	Go to Local
SDC	Select Device Clear
PPC	Parallel Poll Configure
GET	Group Execute Trigger
TCT	Take Control
LLO	Local Lockout
(ACG)	Addressed Command Group
(UCG)	Universal Command Group
(LAG)	Listen Address Group
(TAG)	Talk Address Group
(PCG)	Primary Command Group
(SGG)	Secondary Command Grout
DCL	Device Clear
PPU	Parallel Poll Unconfigure
SPE	Serial Poll Enable
SPD	Serial Poll Disable
UNL	Unlisten
UNT	Untalk

Table of Interface Message Group

DIO8	DIO7	DIO6	DIO5	DIO4	DIO3	DIO2	DIO1	Interface message group (G)
×	0	0	0	b_4	b_3	b_2	b_1	Addressed command G
×	0	0	1	b_4	b_3	b_2	b_1	Universal command G
×	0	1	b_5	b_4	b_3	b_2	b_1	Listen address G
×	0	1	1	1	1	1	1	Unlisten (UNL)
×	1	0	b_5	b_4	b_3	b_2	b_1	Talker address G
×	1	0	1	1	1	1	1	Untalk (UNT)
×	1	1	b_5	b_4	b_3	b_2	b_1	Secondary command G

Table of Address Assignments

Address character		Address switch setting					Primary address	Factory address set device
Talk	Listen	5	4	3	2	1		
b_7 b_6	b_7 b_6	b_5	b_4	b_3	b_2	b_1		
1 0	0 1	↓	↓	↓	↓	↓	10 Decimal	
@	SP	0	0	0	0	0	0	
A	!	0	0	0	0	1	1	
B	"	0	0	0	1	0	2	
C	#	0	0	0	1	1	3	
D	$	0	0	1	0	0	4	
E	%	0	0	1	0	1	5	
F	&	0	0	1	1	0	6	
G	'	0	0	1	1	1	7	
H	(	0	1	0	0	0	8	
I	)	0	1	0	0	1	9	
J	*	0	1	0	1	0	10	
K	+	0	1	0	1	1	11	
L	,	0	1	1	0	0	12	
M	−	0	1	1	0	1	13	Printer Plotter
N	.	0	1	1	1	0	14	
O	/	0	1	1	1	1	15	
P	0	1	0	0	0	0	16	
Q	1	1	0	0	0	1	17	
R	2	1	0	0	1	0	18	
S	3	1	0	0	1	1	19	
T	4	1	0	1	0	0	20	
U	5	1	0	1	0	1	21	
V	6	1	0	1	1	0	22	
W	7	1	0	1	1	1	23	
X	8	1	1	0	0	0	24	
Y	9	1	1	0	0	1	25	
Z	:	1	1	0	1	0	26	
[	;	1	1	0	1	1	27	
\	<	1	1	1	0	0	28	
]	=	1	1	1	0	1	29	
^	>	1	1	1	1	0	30	
?	—	1	1	1	1	1	31	UNL,UNT

(Blank)

APPENDIX B COMPARISON TABLE OF CONTROLLERS' GPIB INSTRUCTIONS

Function	Controller			
	PACKET V (Anritsu)	PC9800 (NEC)	IBM-PC	HP9000 series
Outputs data to a device	WRITE @ device number:data	PRINT @ listener address; data	CALL IBWRT( )	OUTPUT device selector;data
Output binary data to a device	BIN WRITE @ device number:data	WBYTE command; data		
Assigns data entered from a device to a variable	READ @ device number: variable	INPUT @ talker address,listener address;variable LINE INPUT @ talker address,listener address;variable	CALL IBRD( )	ENTER device selector; variable
Assigns binary data entered from a device to a variable	BIN READ @ device number: variable	RBYTE command;variable		
Initializes an interface	IFC @ select code	ISET IFC	CALL IBSIC( )	ABORT select code
Turns REN line on	REN @ select code	ISET REN	CALL IBSRE( )	REMOTE device selector (select code)
Turns REN line off	LCL @ select code (sets all devices local) LCL @ device number (sets only specified devices to listeners, and sends out GTL command)	IRESET REN WBYTE &H3F,listener address, secondary address, &HØ1;	CALL IBSRE( ) CALL IBLOC( )	LOCAL device selector (select code) LOCAL device selector (select code + primary address)

Function	Controller			
	PACKET V (Anritsu)	PC9800 (NEC)	IBM-PC	HP9000 series
Outputs interface message(s) and data	COMMAND @ select code: character string for message [;data]		CALL IBCMD( ) CALL IBCMDA( ) (asynchronous)	SEND select code;message string
Triggers a specified device	TRG @ device number	WBYTE &H3F, listener address, secondary address, &HØ8;	CALL IBTRG( )	TRIGGER device selector
Initializes devices	DCL @ select code (all devices bearing a specified select code) DCL @ device number (specified devices only)	WBYTE &H3F,&H14; WBYTE &H3F, listener address, secondary address,&HØ4;	 CALL IBCLR( )	CLEAR device selector (select code) CLEAR device selector (select code + primary address)
Disables a device from being switched over from remote to local	LLO @ select code	WBYTE &H3F,&H11;		LOCAL LOCKOUT
Transfers control to a specified device	PCT @ device number	WBYTE talker address,&HØ9;	CALL IBPCT ( )	PASS CONTROL
Sends out a service request	SRQ @ select code	ISET SRQ	CALL IBRSV( )	REQUEST select code
Performs serial polling	STATUS @ device number	POLL	CALL IBRSP( )	SPOLL (device selector) (function)
Sets a terminator code	TERM IS	CMD DELIM	CALL IBEOS( ) CALL IBEOT( )	
Sets a limit value for checking a timeout		CMD TIMEOUT	CALL IBTOM( )	

Anritsu

ANRITSU CORPORATION
5-10-27, Minamiazabu, Minato-ku, Tokyo, 106 Japan
PHONE. 03-3446-1111
TELEX J 34372 ANRITU

MP MASTER
MA28380